


=====  
Acq. Operator :  
Acq. Instrument : HPLC  
Sample Name : M3095-Tubastatin A-03

Seq. Line : 1  
Location : Vial 24  
Inj : 1

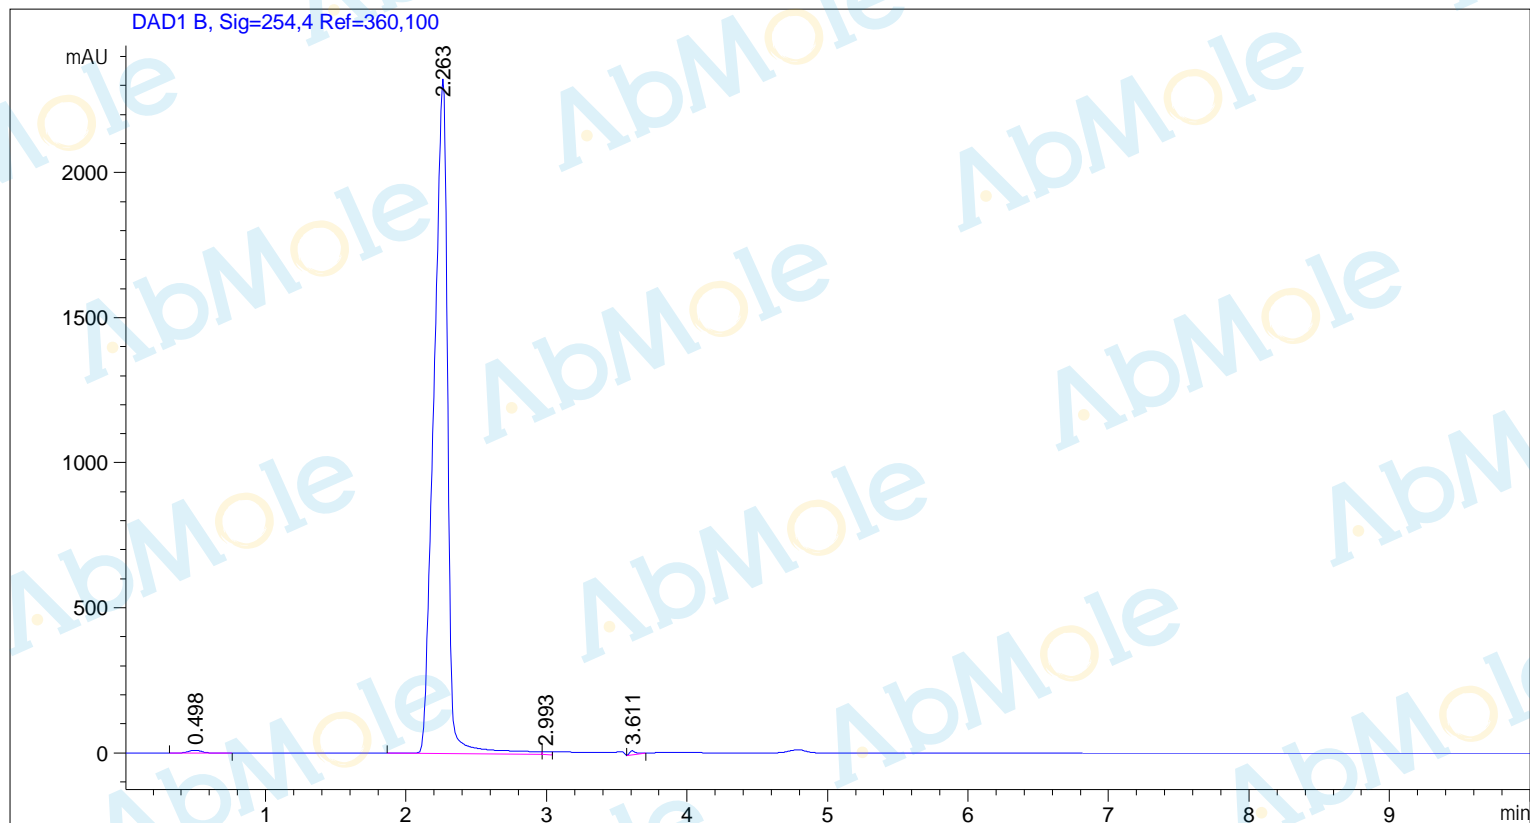

=====  
Area Percent Report  
=====

Sorted By : Signal  
Multiplier: : 1.0000  
Dilution: : 1.0000  
Use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 B, Sig=254, 4 Ref=360, 100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	0.498	BB	0.0974	60.33745	9.59617	0.3799
2	2.263	BV	0.1029	1.57406e4	2326.23389	99.0975
3	2.993	VV	0.0603	41.59692	10.05176	0.2619
4	3.611	BB	0.0452	41.42234	13.74778	0.2608

Totals : 1.58840e4 2359.62959

=====  
\*\*\* End of Report \*\*\*