

Data file: C:\CHEM32\1\DATA\M31233-02Final.D

Sample name: M31233- ω -Agatoxin IVA-02

Description: Mobile Phase: Buffer A: 0.1% TFA in H₂O
Buffer B: 0.1% TFA in ACN
Gradient: 27-37%B in 20min, Flow rate: 1.0ml/min
Column: Unitary C18 5 μ m 100A 4.6*150mm
Instrument: Agilent HPLC 1100

Instrument:


1100

Location: 31

Injection: 1 of 1

Injection volume: 20.000

Acq.operator: System

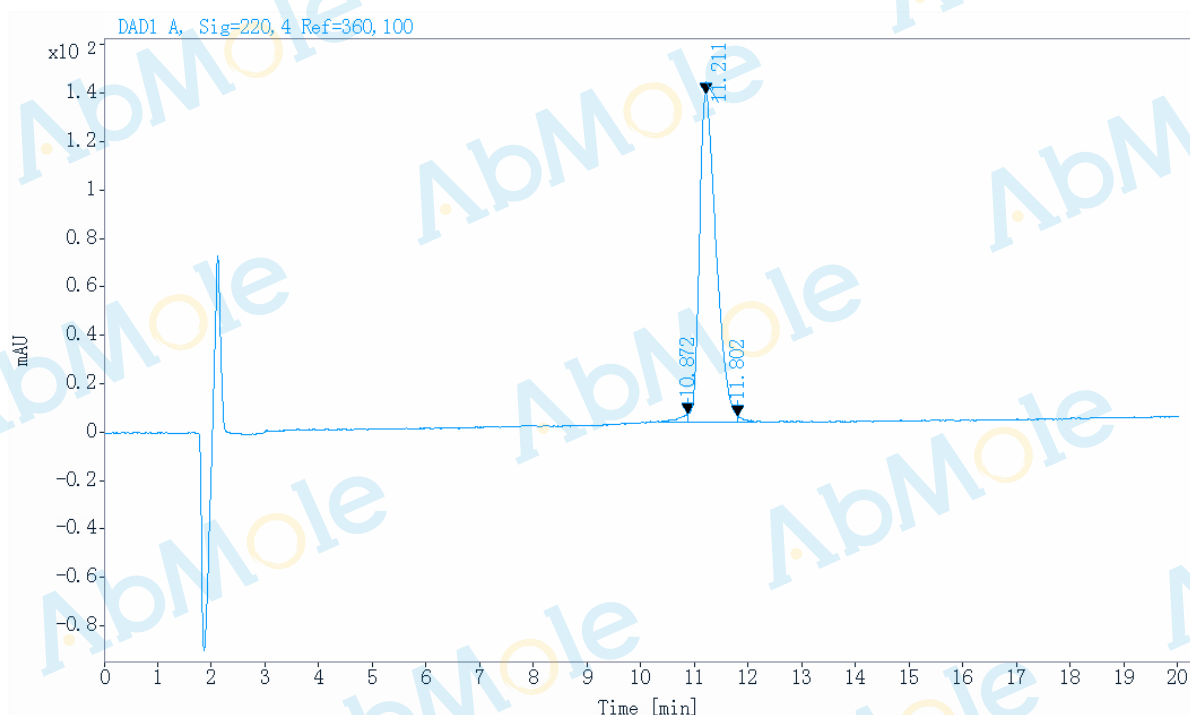

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT[min]	Type	Width[min]	Area	Height	Area%	Name
10.872	MF	0.2025	38.4645	3.1664	1.2891	
11.211	MF	0.3601	2928.2166	135.5143	98.1387	
11.802	FM	0.1293	17.0717	2.2012	0.5722	
Sum			2983.7528			