


=====

Acq. Operator	: System	Seq. Line	: 5
Acq. Instrument	: LC1260	Location	: Vial 12
		Inj	: 1
		Inj Volume	: 0 µl
Different Inj Volume from Sequence !		Actual Inj Volume	: 2 µl
Acq. Method	: E:\DATA\Data\10-90 AD 220 15MIN.M		

=====

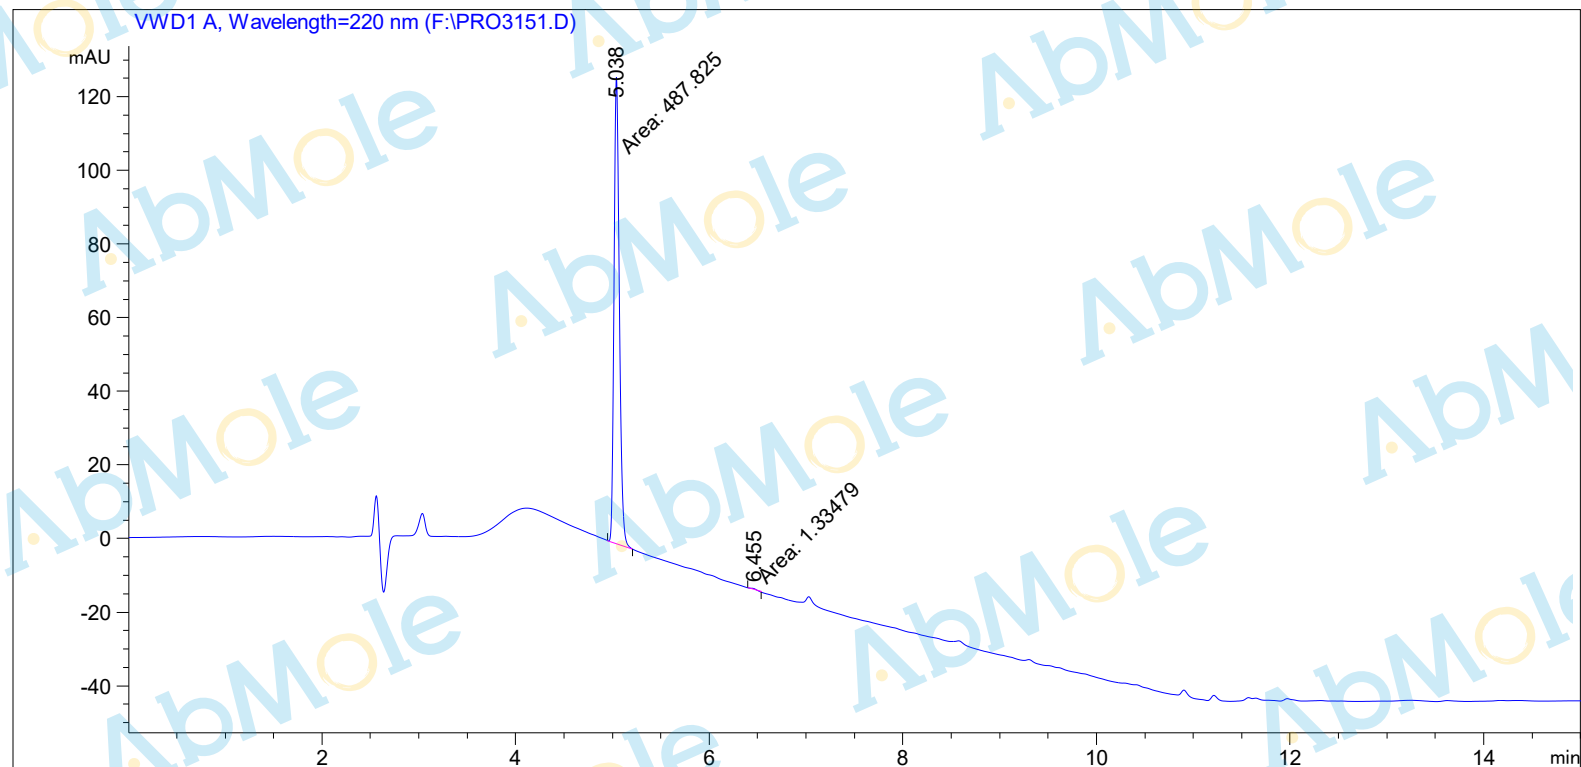

=====

Area Percent Report

=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=220 nm

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	5.038	MM	0.0641	487.82492	126.81822	99.7271
2	6.455	MM	0.0666	1.33479	3.33959e-1	0.2729

Totals : 489.15971 127.15218

=====
*** End of Report ***