


=====
Acq. Operator : admin
Sample Operator : M3283-Pioglitazone-01
Acq. Instrument : 3

Location : P2-E-07
Inj : 1
Inj Volume : 0.100 µl
Actual Inj Volume : 4.000 µl

Different Inj Volume from Sample Entry!

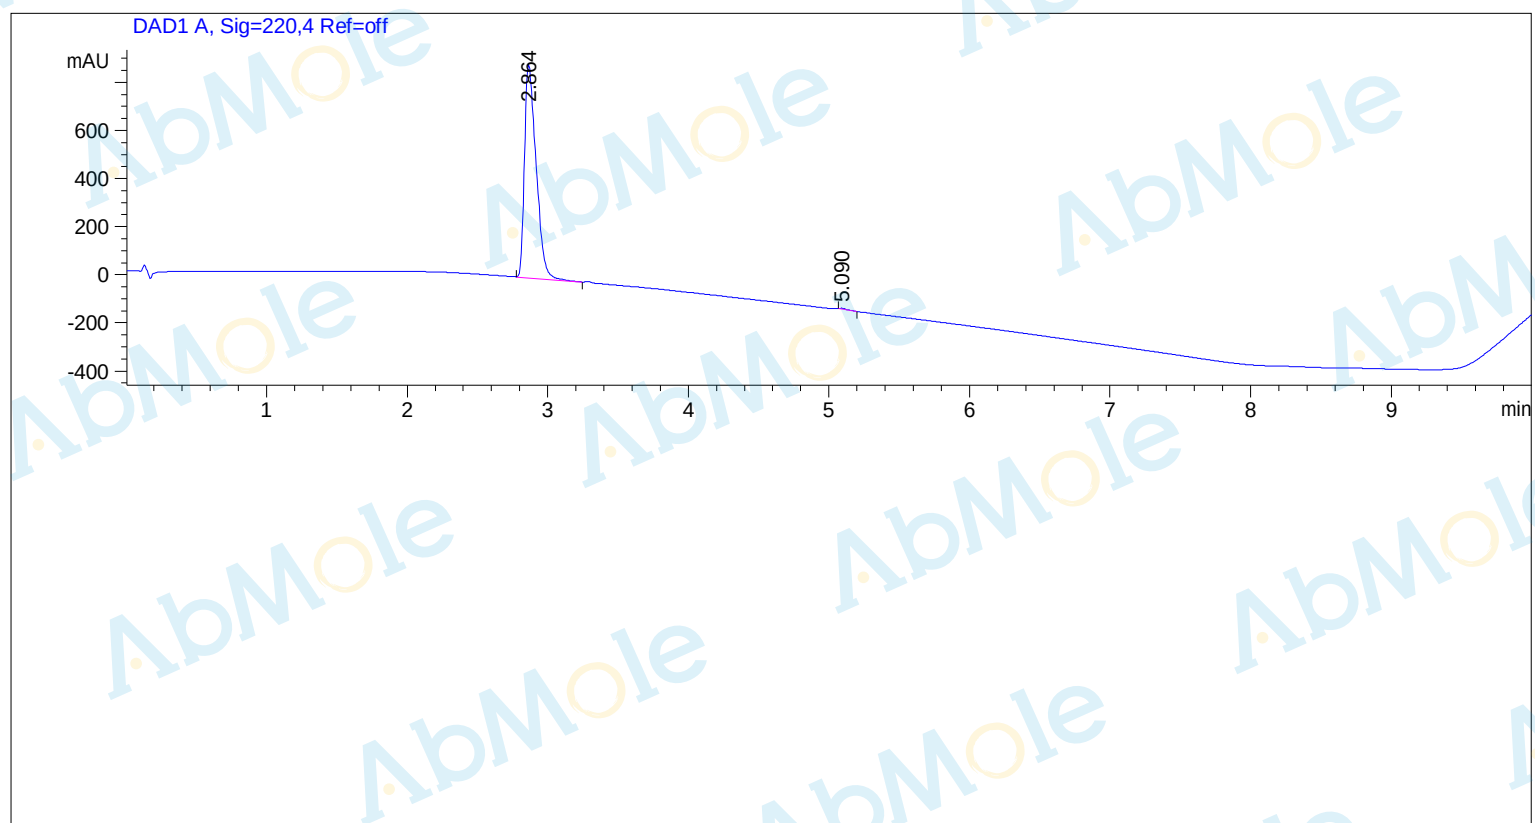

=====
Area Percent Report
=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 A, Sig=220,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	2.864	BB	0.0872	5100.94482	886.08167	99.7674
2	5.090	BB	0.0524	11.89012	3.27366	0.2326

Totals : 5112.83494 889.35533