



Agilent Technologies

Sample name: M3372-Clonidine hydrochloride-02

Injection date:

Instrument: A012

Location:

Inj. volume: 2


Type:

Acq. method: HPLC

Sample amount:

Processing method:

Manually modified:

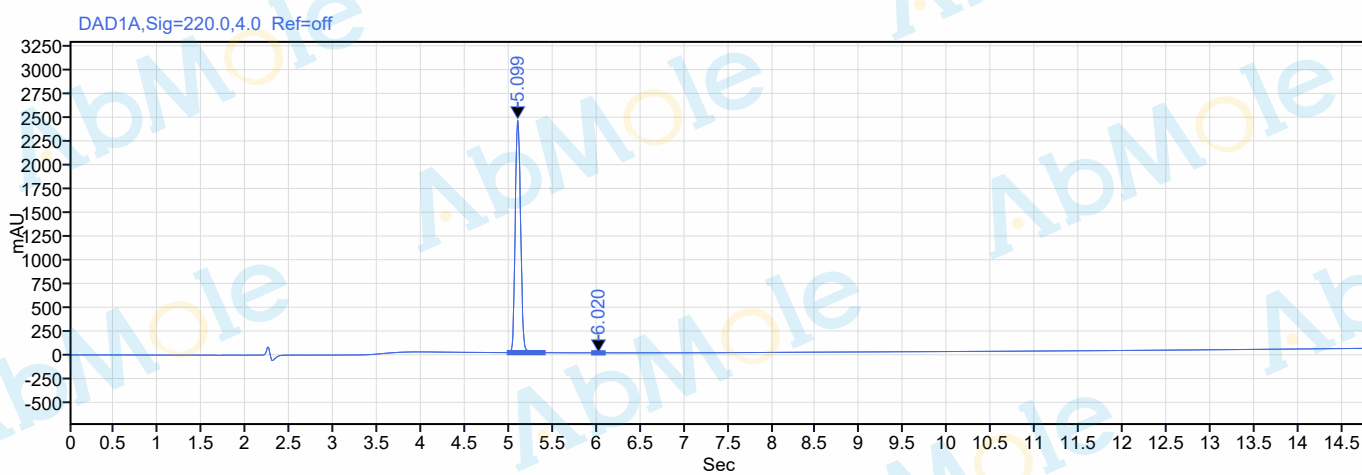

Signal: DAD1A, Sig=220.0, 4.0 Ref=off

RT [min]	Peak Resolution USP	Area	Height	Area%
5.099		10530.6	2454.4	99.946
6.020		5.7	1.9	0.054