



Agilent Technologies

Sample name: M3645-MG149-02

Instrument: A010

Inj. volume: 3

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

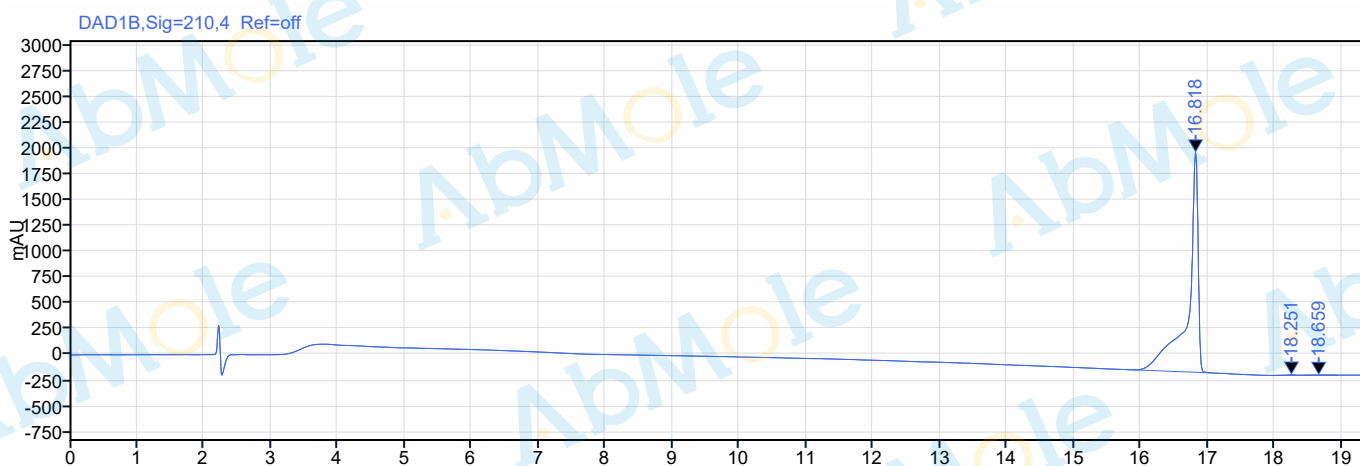

Signal: DAD1B,Sig=210,4 Ref=off

RT [min]	Area	Height	Peak Resol ution USP	Area%
16.818	22352.00	2134.05		99.71
18.251	36.10	5.45		0.16
18.659	28.73	1.53		0.13
Sum	22416.82			