



Agilent Technologies

Sample name: M3671-Cyclophosphamide monohydrate-01

Injection date:

Instrument: 3

Location:

Inj. volume: HPLC


Type:

Acq. method:

Sample amount:

Processing method:

Manually modified:

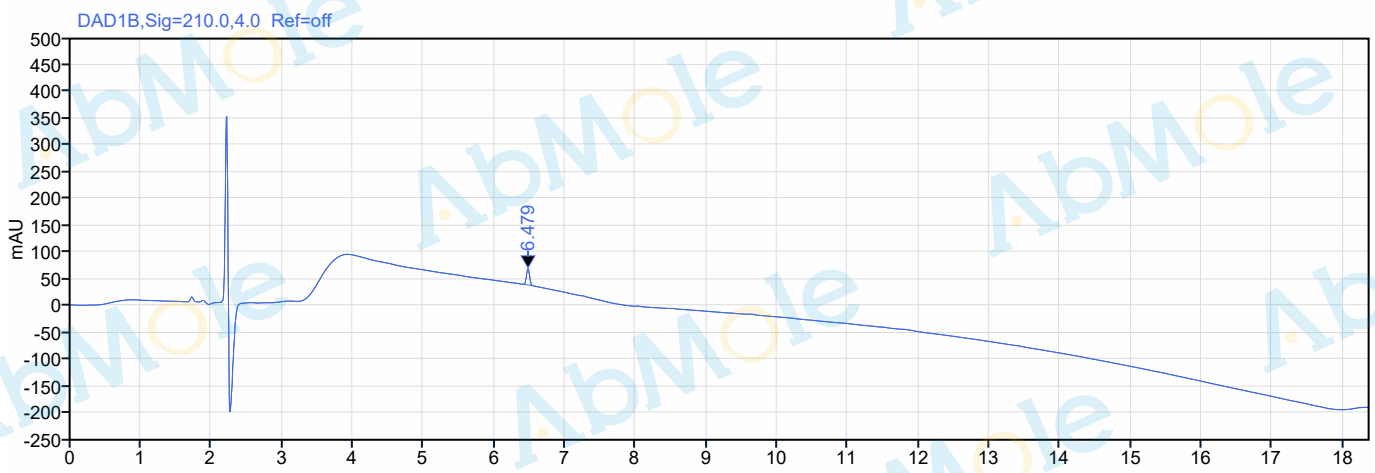

Signal: DAD1B,Sig=210.0,4.0 Ref=off

RT [min]	Area	Height	Area%
6.479	92.78	30.51	100.00
Sum	92.78		