


=====  
Acq. Operator : SYSTEM  
Acq. Instrument : 0  
Sample Name : M3938-Baicalin-02

Seq. Line : 1  
Location : P2-D-03  
Inj : 1  
Inj Volume : 1.000 µl

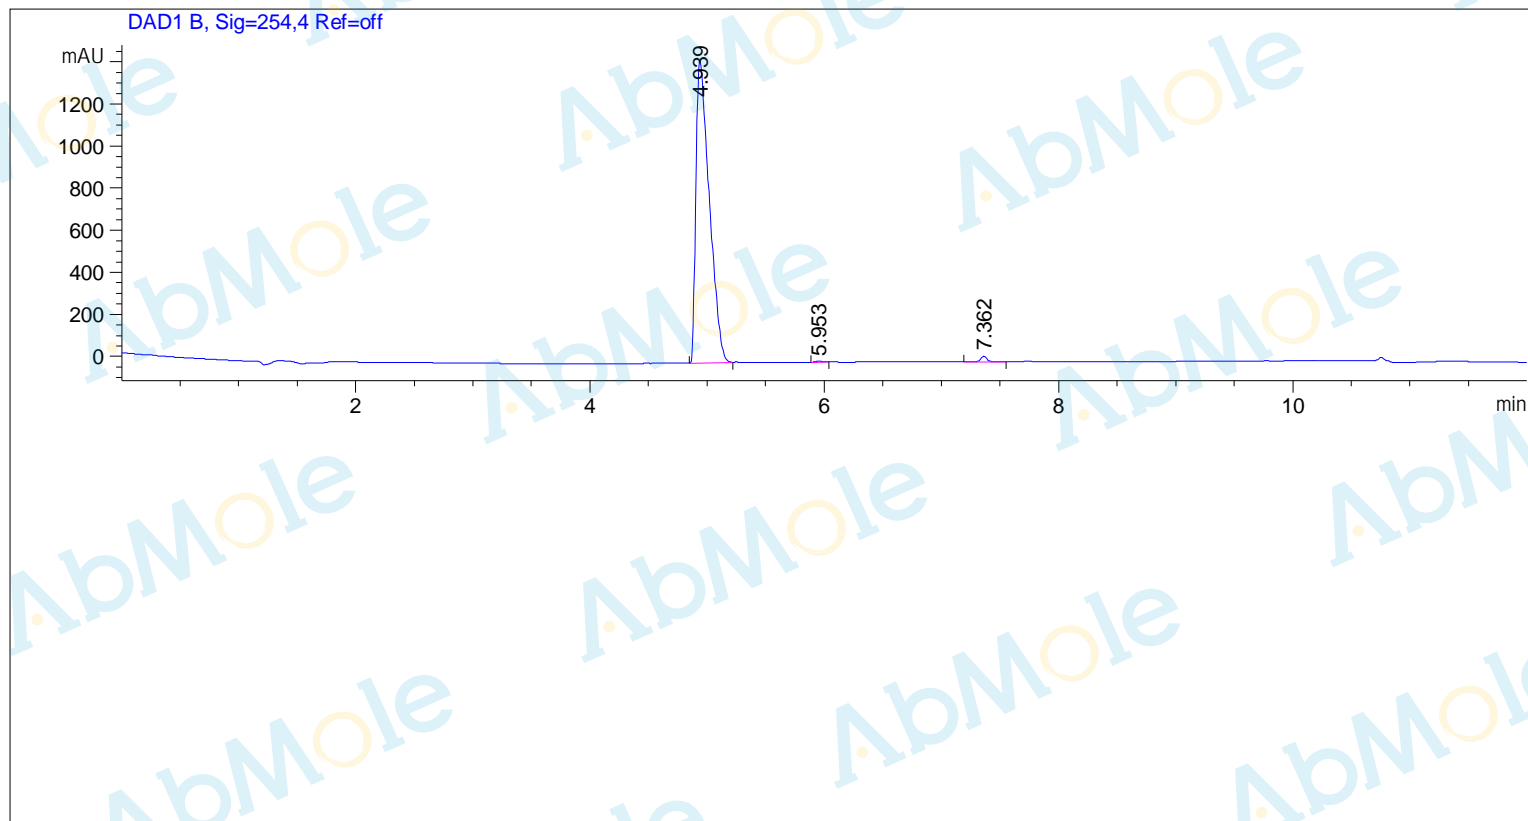

=====  
Area Percent Report  
=====

Sorted By : Signal  
Multiplier : 1.0000  
Dilution : 1.0000  
Use Multiplier & Dilution Factor with ISTDs

Signal 2: DAD1 B, Sig=254,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	4.939	BB	0.1138	1.13575e4	1442.93005	98.9495
2	5.953	BB	0.0596	18.52327	4.74246	0.1614
3	7.362	BB	0.0581	102.05878	27.00926	0.8892

Totals : 1.14781e4 1474.68177