



Agilent Technologies

Sample name: M40499-BI-2865-01

Instrument: A010

Inj. volume: 1

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

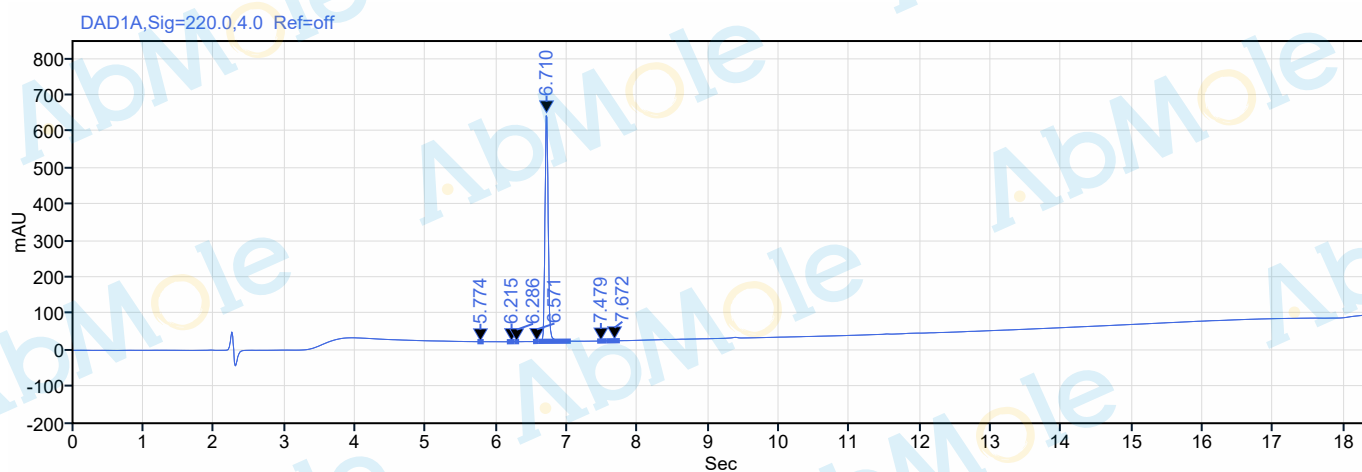

Signal: DAD1A,Sig=220.0,4.0 Ref=off

RT [min]	Peak Resolution USP	Area	Height	Area%
5.774		0.7	0.2	0.034
6.215		1.9	0.7	0.094
6.286		0.2	0.1	0.009
6.571		0.8	0.3	0.042
6.710		1994.1	625.4	99.109
7.479		1.7	0.4	0.083
7.672		12.7	3.3	0.629