



Agilent Technologies

Sample name: M40519-AOH1996-03

Instrument: A010

Inj. volume: 2

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

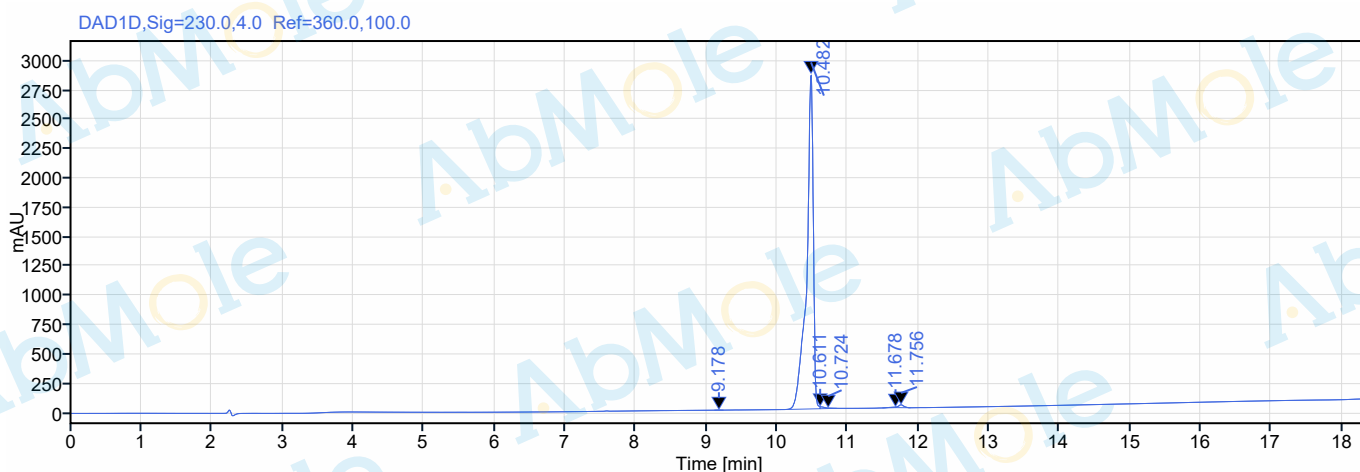

Signal: DAD1D,Sig=230.0,4.0 Ref=360.0,100.0

RT [min]	Type	Width [min]	Area	Height	Area%
9.178	MM m	0.13	2.64	0.75	0.01
10.482	BM m	0.51	18820.13	2851.20	98.72
10.611	MM m	0.11	69.94	17.53	0.37
10.724	MM m	0.13	14.58	4.07	0.08
11.678	MM m	0.19	27.07	4.87	0.14
11.756	MB m	0.21	129.11	24.10	0.68