



Agilent Technologies

Sample name: M4245-Schizandrin-B-02

Instrument: A012

Inj. volume: 5

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

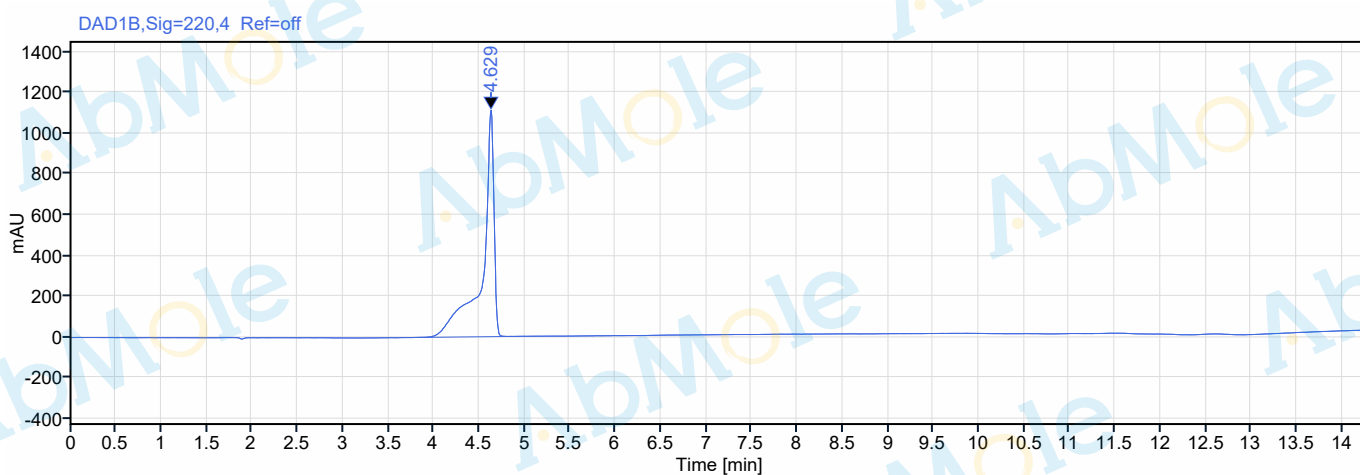

Signal: DAD1B,Sig=220,4 Ref=off

RT [min]	Area	Height	Area%
4.629	9927.88	1111.93	100.00