



Sample name: M4433-Alantolactone-03

Injection date:

Instrument: A012

Location:

Inj. volume: 3


Type:

Acq. method: HPLC

Sample amount:

Processing method:

Manually modified:

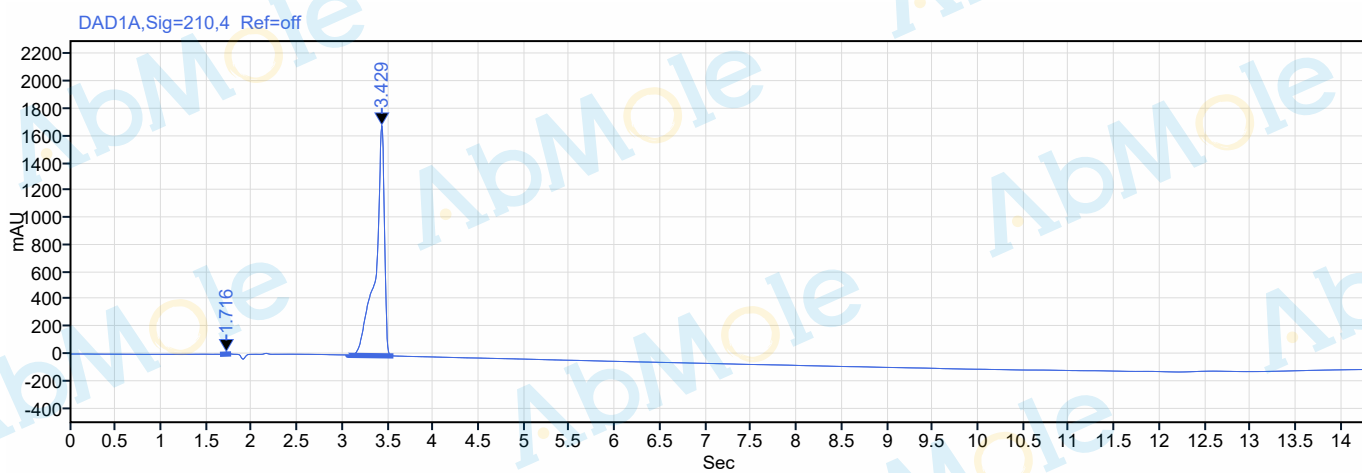

Signal: DAD1A, Sig=210,4 Ref=off

RT [min]	Peak Resolution USP	Area	Height	Area%
1.716		46.9	13.4	0.402
3.429		11616.6	1690.8	99.598