



Sample name: M4460-Oroxylin-A-01

Instrument: A010

Inj. volume: 1.5

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

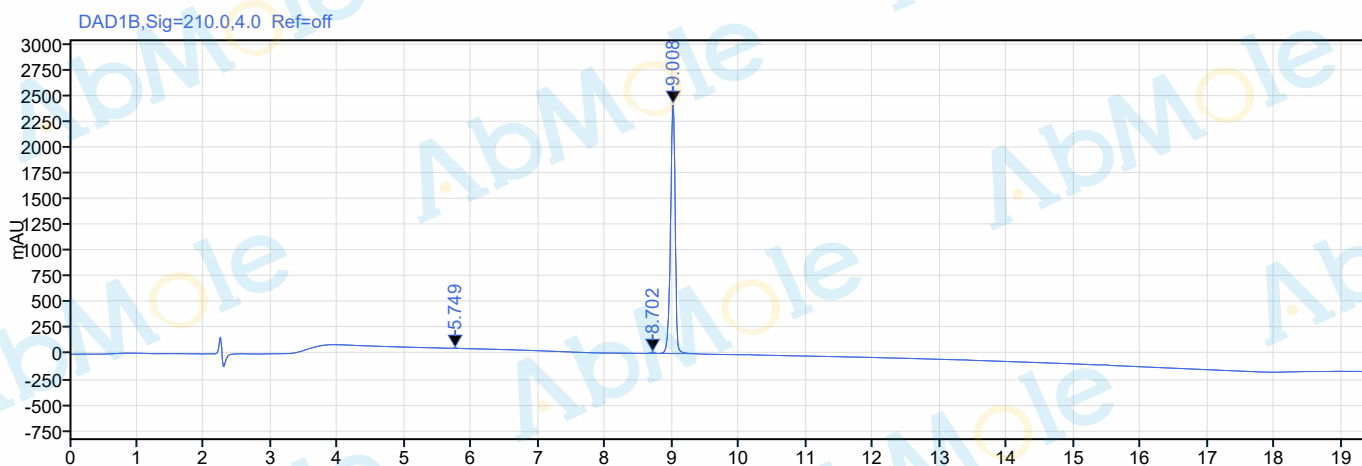

Signal: DAD1B, Sig=210.0,4.0 Ref=off

RT [min]	Area	Height	Peak Resolution USP	Area%
5.749	11.63	4.31		0.10
8.702	50.34	13.86		0.43
9.008	11594.32	2425.72		99.47