




Sample name: M4552-Nobiletin-03
Instrument: 2
Inj. volume: HPLC
Acq. method:
Processing method:
Manually modified:

Injection date:
Location:
Type:
Sample amount:

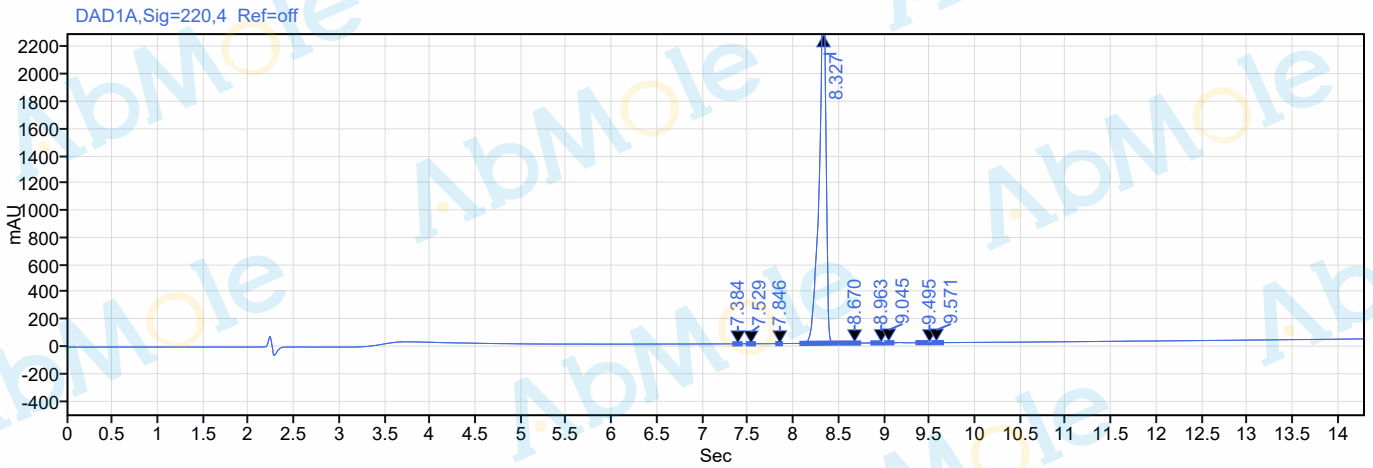

Signal: DAD1A,Sig=220,4 Ref=off

RT [min]	Peak Resolution USP	Area	Height	Area%
7.384		4.1	1.4	0.030
7.529		1.2	0.4	0.009
7.846		0.9	0.3	0.006
8.327		13604.0	2594.9	99.252
8.670		15.0	3.7	0.110
8.963		14.1	3.2	0.103
9.045		31.9	7.8	0.232
9.495		7.3	1.4	0.053
9.571		28.1	6.4	0.205