



Agilent Technologies

Sample name: M4570-Palmatine-02

Instrument: A010

Inj. volume: 2

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

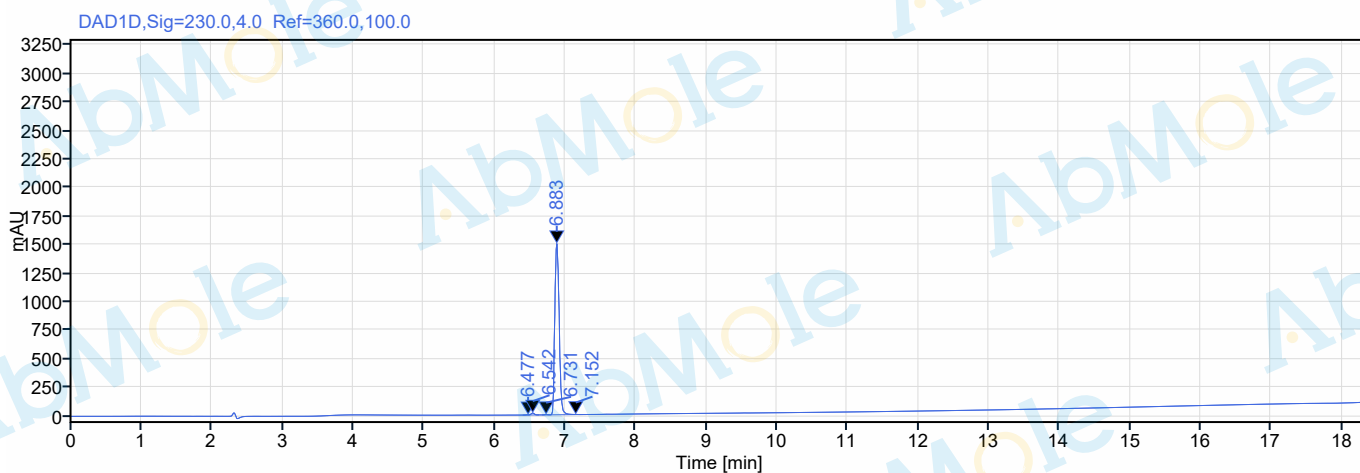

Signal: DAD1D,Sig=230.0,4.0 Ref=360.0,100.0

RT [min]	Type	Width [min]	Area	Height	Area%
6.477	MM m	0.09	3.96	1.62	0.06
6.542	MM m	0.14	52.40	16.76	0.80
6.731	BB	0.11	6.17	2.17	0.09
6.883	BV	0.35	6466.01	1499.24	98.98
7.152	VB	0.10	4.15	1.20	0.06