



Agilent Technologies

Sample name: M4691-Lycorine hydrochloride-04

Injection date:

Instrument: A012

Location:

Inj. volume: 2


Type:

Acq. method: HPLC

Sample amount:

Processing method:

Manually modified:

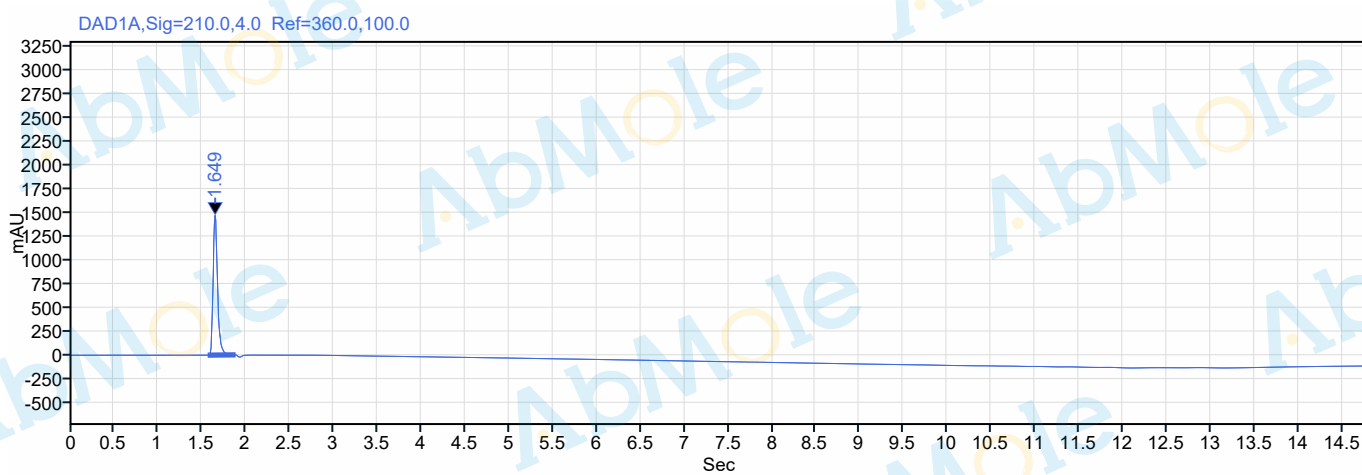

Signal: DAD1A, Sig=210.0, 4.0 Ref=360.0, 100.0

RT [min]	Peak Resolution USP	Area	Height	Area%
1.649		5243.2	1470.4	100.000