




Sample name: M4973-BAPTA-AM-03  
Instrument: 3  
Inj. volume: HPLC  
Acq. method:  
Processing method:  
Manually modified:

Injection date:  
Location:  
Type:  
Sample amount:

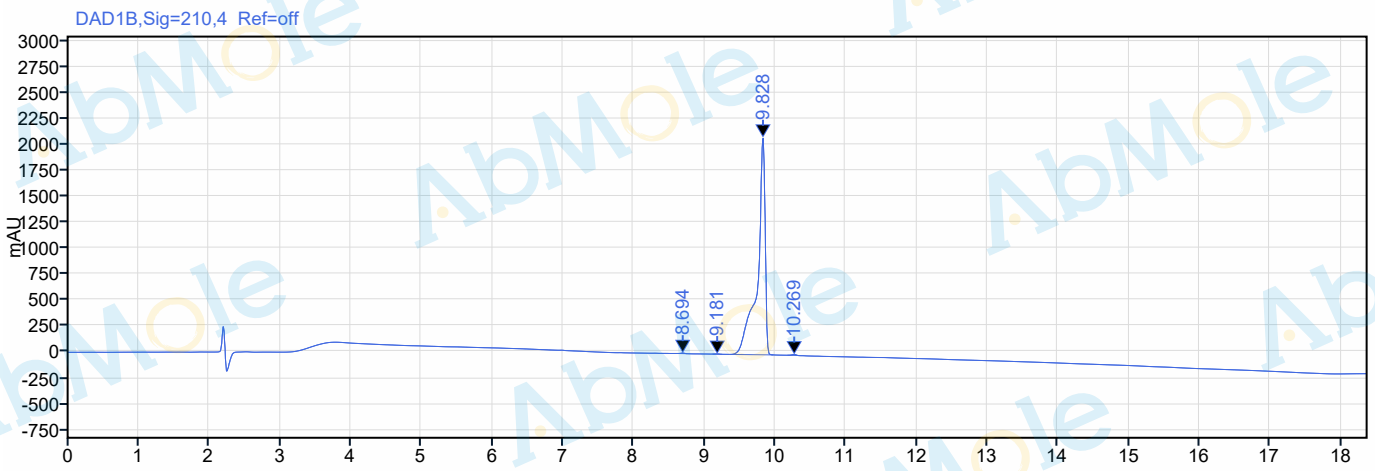

Signal: DAD1B, Sig=210,4 Ref=off

RT [min]	Area	Height	Area%
8.694	18.06	5.28	0.11
9.181	9.71	2.72	0.06
9.828	15962.54	2097.75	99.60
10.269	36.84	9.47	0.23
Sum	16027.15		