


AbMole

Data file: D:\CHEM32\1\DATA\240625\20240625 2024-06-25 09-20-22\M49831
24020004Final.D
Sample name: M49831-Melanotan I-03
Description: Mobile phase: Buffer A: 0.1%TFA in H2O
Buffer B: 0.1%TFA in ACN
Gradient: 22-32% B in 20min , Flow rate: 1.0ml/min
Column: Uni tary C18, 4. 6*150mm, 5um 100A
Instrument: Agilent HPLC 1100

Instrument: 1100 Location: 44
Injection date: 2024/6/25 10: 42: 04 Injection: 1 of 1
Last changed: 2024/6/25 10: 03: 15 Injection volume: 10. 000
Acq. operator: SYSTEM

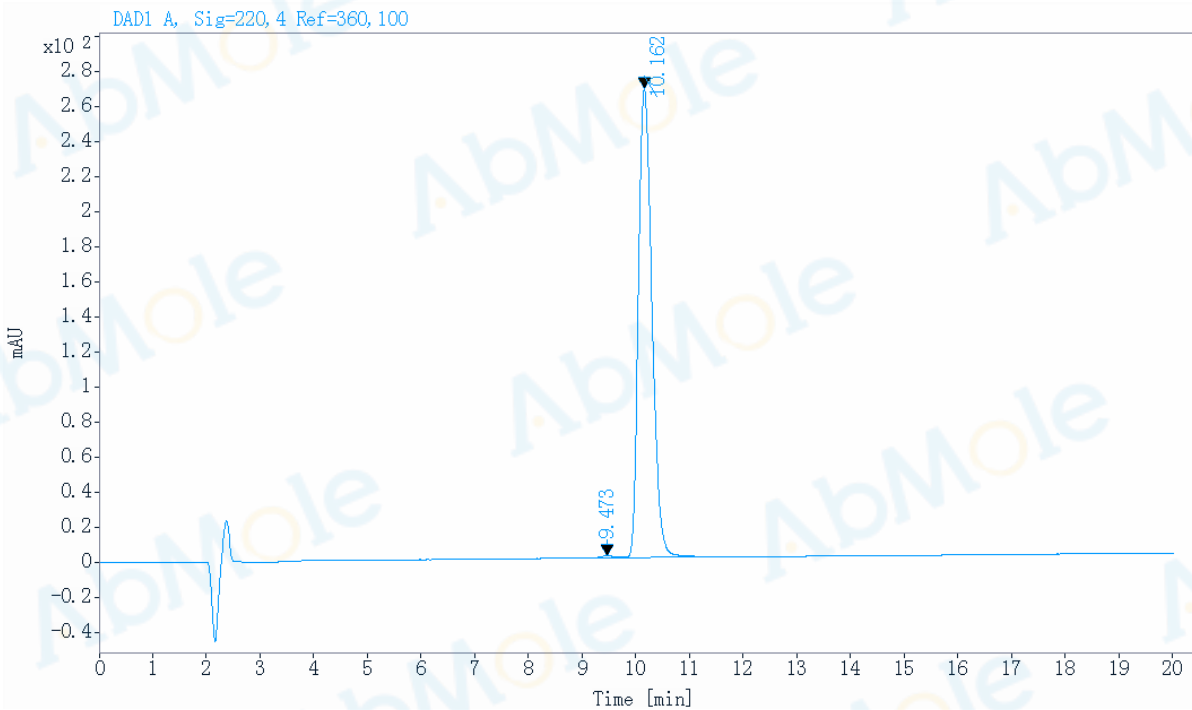

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT[mi n]	Type	Width[mi n]	Area	Height	Area%	Name
9. 473	BV E	0. 3320	26. 9766	1. 1405	0. 5724	
10. 162	VBAR	0. 2777	4686. 3091	265. 8141	99. 4276	
Sum			4713. 2857			