




Agilent Technologies

Sample name: M5015-BPTES-02
Instrument: 10
Inj. volume: HPLC
Acq. method:
Processing method:
Manually modified:

Injection date:
Location:
Type:
Sample amount:

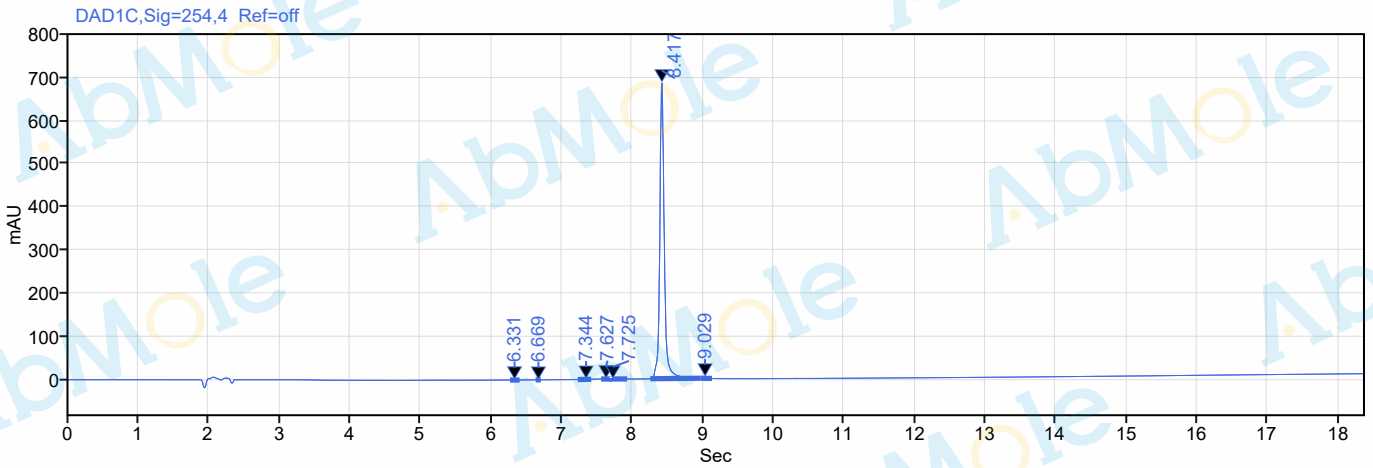

Signal: DAD1C,Sig=254,4 Ref=off

RT [min]	Width [min]	Area	Height	Area%
6.331	0.14	3.1	1.0	0.10
6.669	0.07	0.7	0.3	0.02
7.344	0.19	6.3	1.2	0.20
7.627	0.14	6.1	1.3	0.20
7.725	0.23	5.6	0.7	0.18
8.417	0.71	3065.4	687.2	98.82
9.029	0.16	14.9	4.0	0.48