



Agilent Technologies

Sample name: M5058-Ganciclovir-03

Instrument: A010

Inj. volume: 3

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

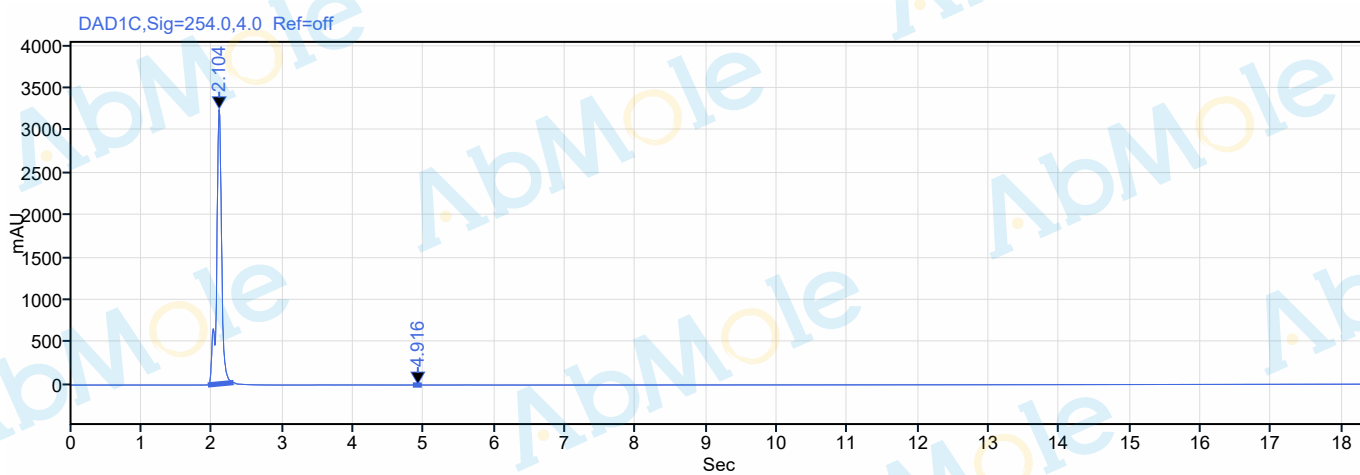

Signal: DAD1C,Sig=254.0,4.0 Ref=off

RT [min]	Peak Resolution USP	Width [min]	Area	Height	Area%
2.104		0.36	16069.1	3237.1	99.96
4.916		0.13	6.2	1.9	0.04