




Sample name: M5400-Alosetron Hydrochloride-01
Instrument: 2
Inj. volume: HPLC
Acq. method:
Processing method:
Manually modified:

Injection date:
Location:
Type:
Sample amount:

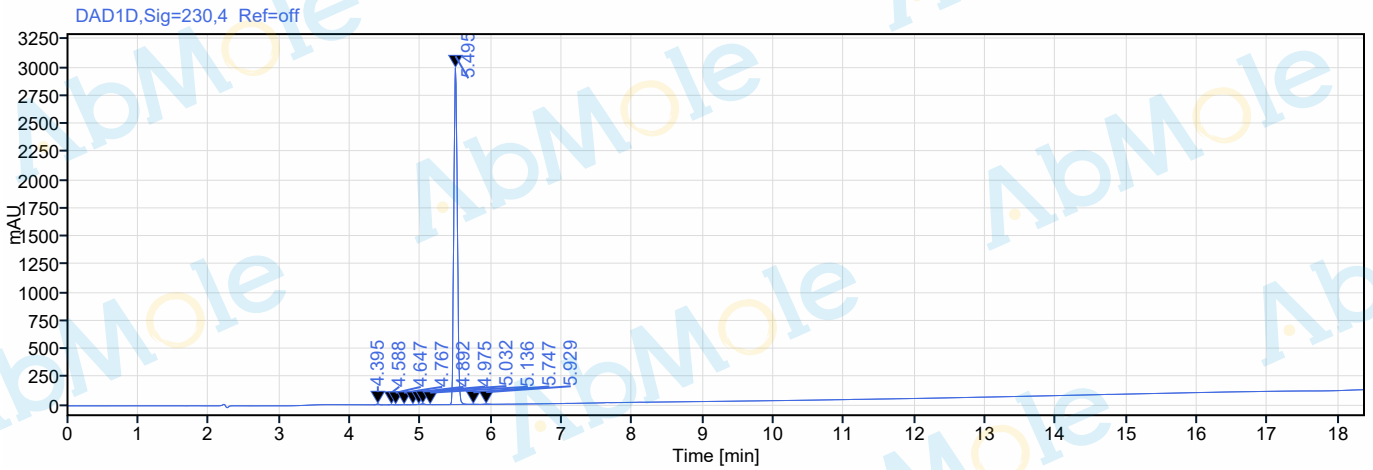

Signal: DAD1D,Sig=230,4 Ref=off

RT [min]	Type	Width [min]	Area	Height	Area%	Name
4.395	MB m	0.05	18.91	6.81	0.18	
4.588	BM m	0.05	6.36	2.21	0.06	
4.647	MM m	0.04	1.44	0.56	0.01	
4.767	MM m	0.06	3.12	0.88	0.03	
4.892	MM m	0.05	0.98	0.36	0.01	
4.975	MM m	0.03	4.84	2.31	0.05	
5.032	MB m	0.05	23.93	6.89	0.23	
5.136	MM m	0.04	1.49	0.66	0.01	
5.495	BB	0.30	10299.71	2986.72	99.28	
5.747	BB	0.13	4.04	1.40	0.04	
5.929	BM m	0.06	9.56	2.60	0.09	
		Sum	10374.38			