



Agilent Technologies

Injection date:

Sample name: M55306-Guanosine 3',5'-cyclic monophosphate-02

Instrument: A010

Location:

Inj. volume: 6


Type:

Acq. method: HPLC

Sample amount:

Processing method:

Manually modified:

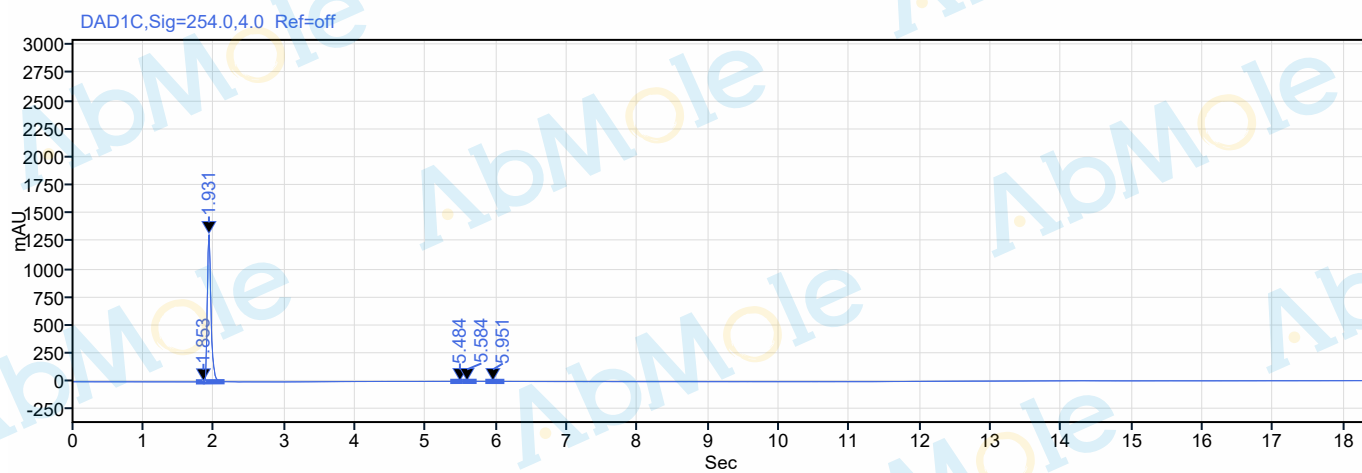

Signal: DAD1C,Sig=254.0,4.0 Ref=off

| RT [min] | Peak Resolution USP | Width [min] | Area   | Height | Area% |
|----------|---------------------|-------------|--------|--------|-------|
| 1.853    |                     | 0.11        | 4.8    | 1.7    | 0.10  |
| 1.931    |                     | 0.29        | 4760.3 | 1316.0 | 99.74 |
| 5.484    |                     | 0.18        | 1.6    | 0.2    | 0.03  |
| 5.584    |                     | 0.19        | 2.9    | 0.5    | 0.06  |
| 5.951    |                     | 0.27        | 3.0    | 0.3    | 0.06  |