



Agilent Technologies

Sample name: M55647-(R)-NX-2127-02

Instrument: A010

Inj. volume: 5

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

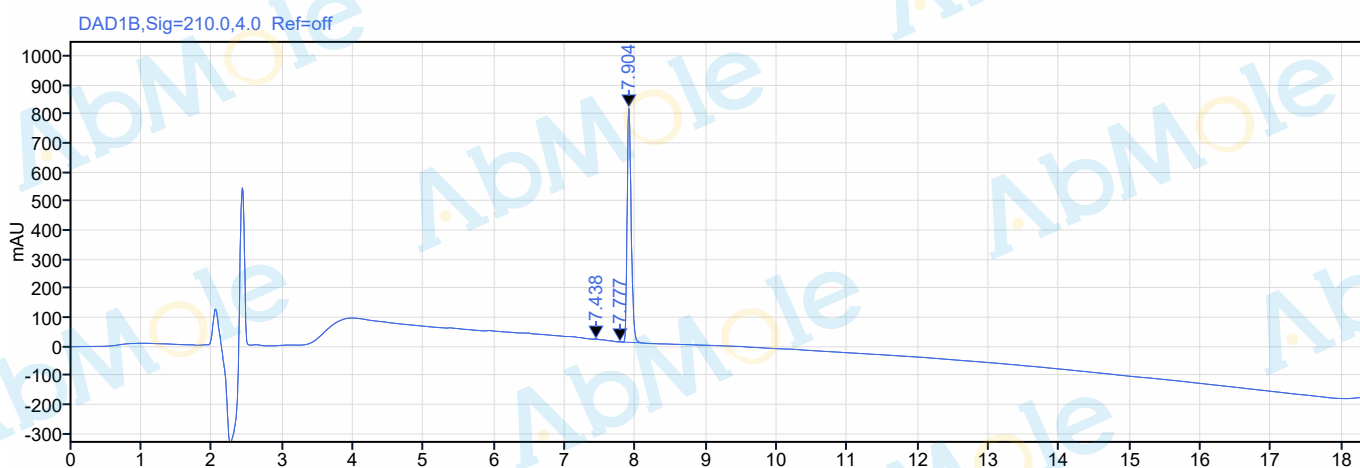

Signal: DAD1B,Sig=210.0,4.0 Ref=off

RT [min]	Area	Height	Peak	Area%
7.438	5.15	1.78		0.16
7.777	2.47	0.87		0.08
7.904	3201.40	806.46		99.76