


=====
Acq. Operator : admin
Sample Operator : M5590-Dopamine HCl-04
Acq. Instrument : LCMS003

Location : P1-E-09
Inj : 1
Inj Volume : 0.100 µl
Actual Inj Volume : 4.000 µl

Different Inj Volume from Sample Entry!

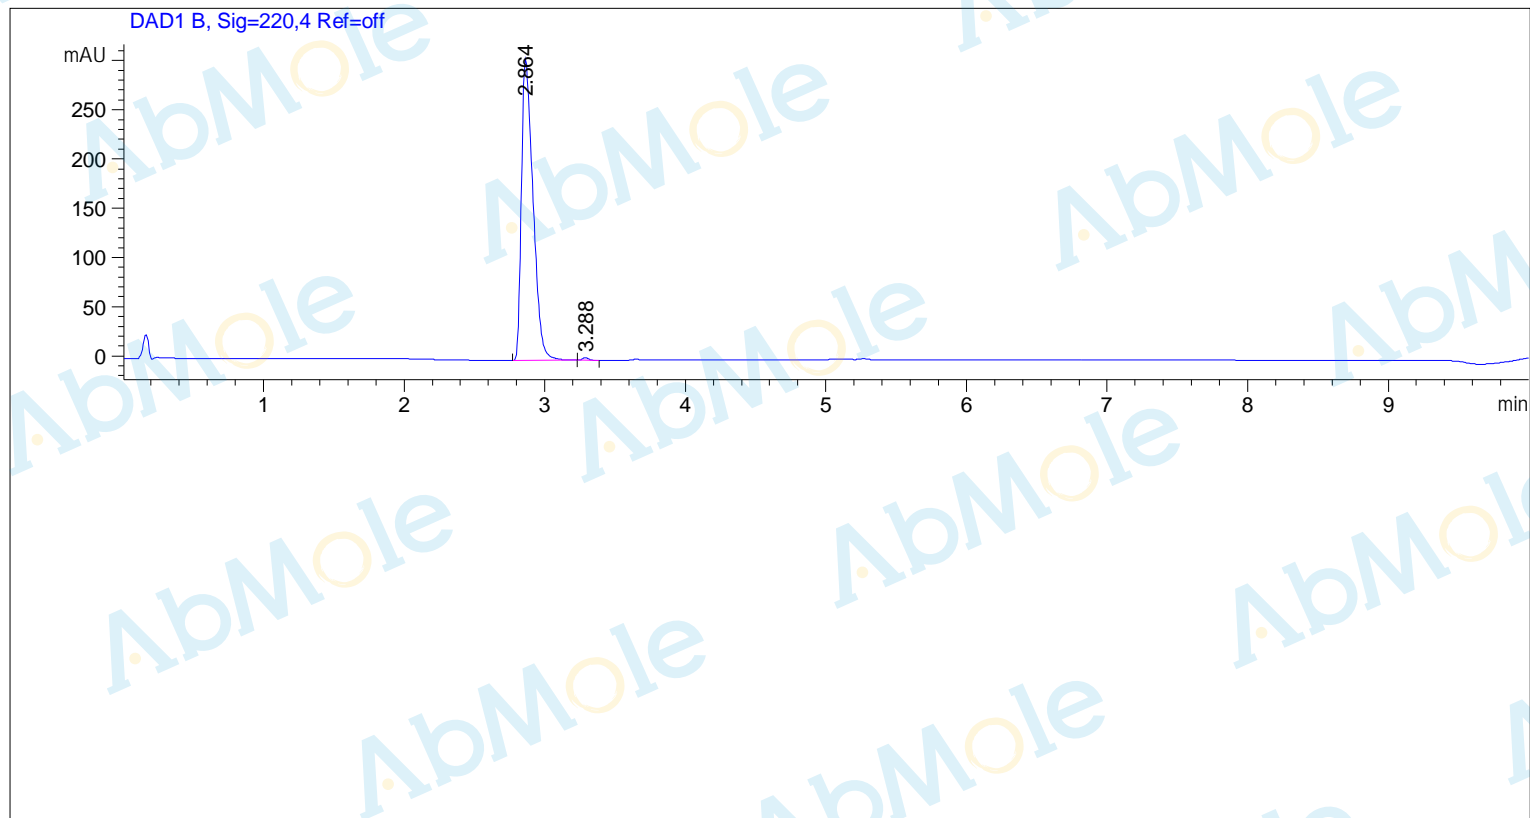

=====
Area Percent Report
=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 A, Sig=220,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	2.864	BB	0.0869	1753.15930	305.92172	99.5804
2	3.288	BB	0.0455	7.38738	2.57475	0.4196

Totals : 1760.54668 308.49647