


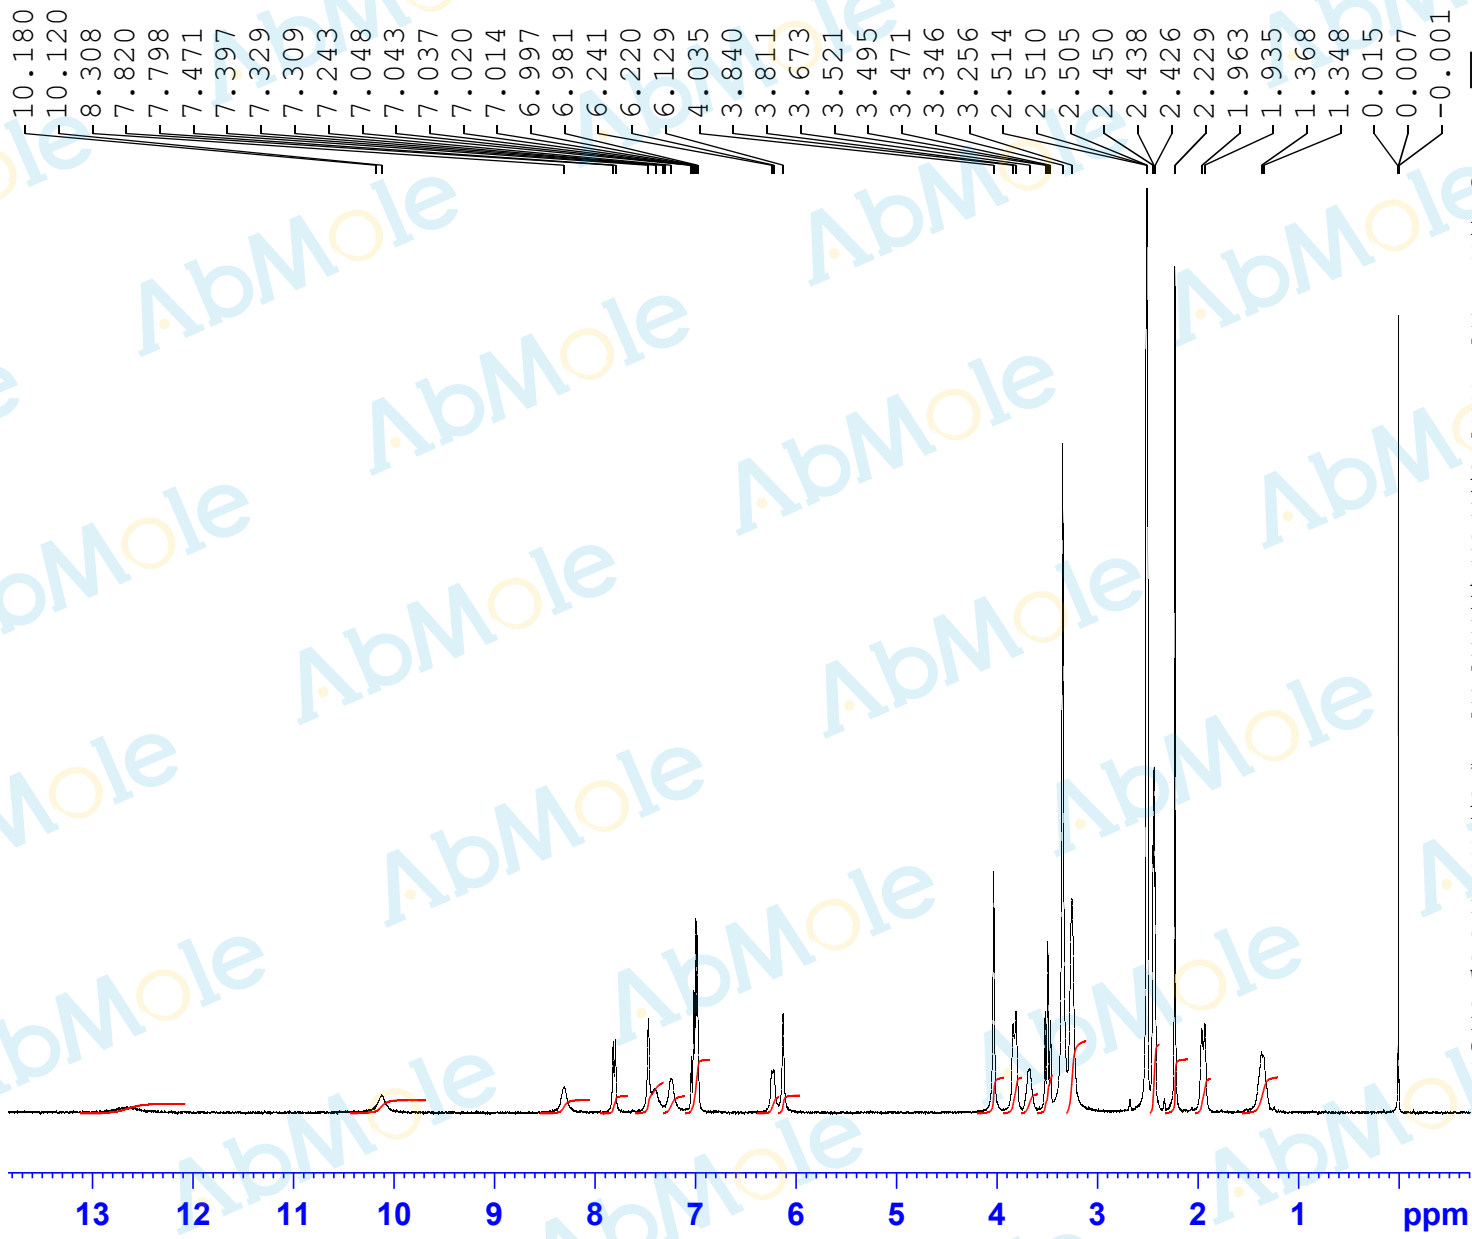

Current Data Parameters
NAME M5613-Entrectinib (RXDX-101)-01
EXPNO 1
PROCNO 1

F2 - Acquisition Parameters
Time 11.55
INSTRUM spect
PROBHD 5 mm PADUL 13C
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.122266 Hz
AQ 4.0894465 sec
RG 199.46
DW 62.400 usec
DE 6.50 usec
TE 294.5 K
D1 1.00000000 sec
TD0 1

===== CHANNEL f1 =====
SFO1 400.1324710 MHz
NUC1 1H
P1 10.00 usec
PLW1 20.00000000 W

F2 - Processing parameters
SI 65536
SF 400.1300000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

13 12 11 10 9 8 7 6 5 4 3 2 1 ppm
0.57 0.77 0.79 1.00 1.78 1.01 3.10 0.95 1.05 2.08 2.08 1.12 2.20 4.19 3.98 3.14 2.01 2.09