



Agilent Technologies

Sample name: M5700-Idasanutlin (RG-7388)-02

Injection date:

Instrument: A010

Location:

Inj. volume: 4


Type:

Acq. method: HPLC

Sample amount:

Processing method:

Manually modified:

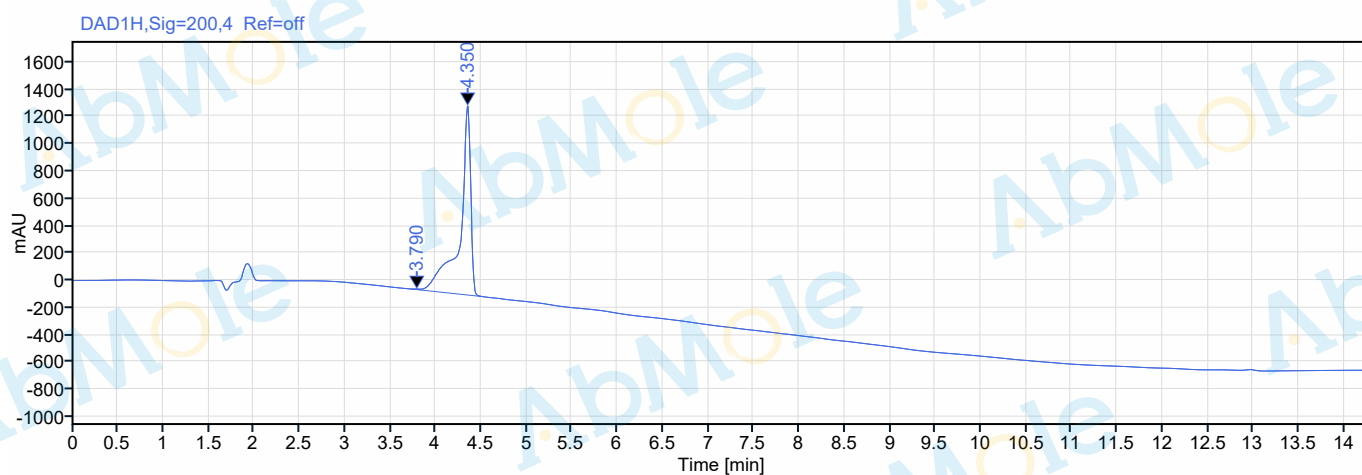

Signal: DAD1H,Sig=200,4 Ref=off

RT [min]	Type	Width [min]	Area	Height	Area%
3.790	MM m	0.10	20.57	4.52	0.18
4.350	MM m	0.68	11517.94	1386.23	99.82