



Agilent Technologies

Sample name: M5791-Mitomycin C-11

Instrument: A010

Inj. volume: 2

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

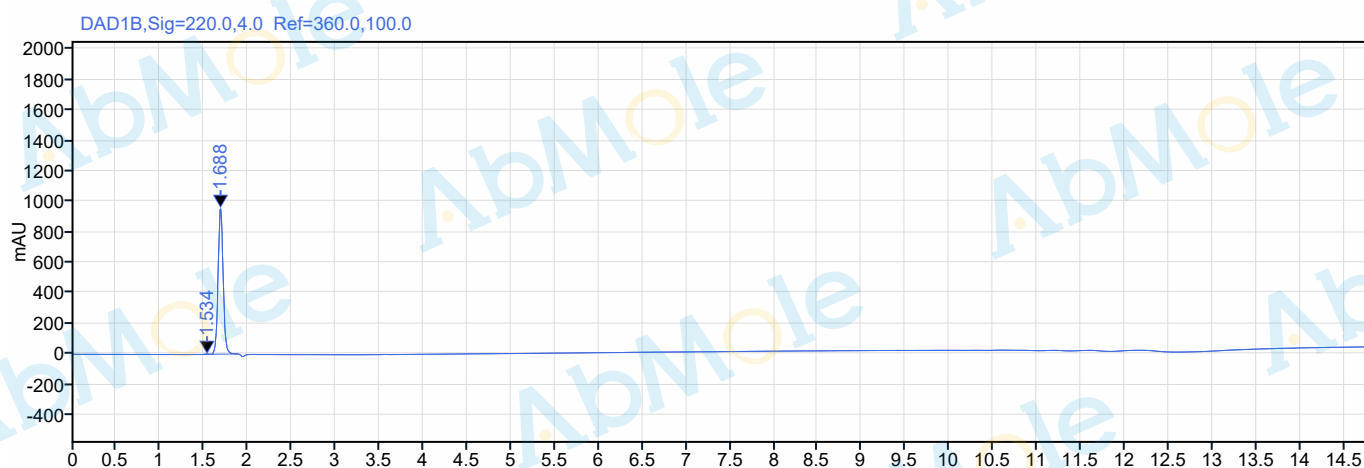

Signal: DAD1B,Sig=220.0,4.0 Ref=360.0,100.0

RT [min]	Area	Height	Area%
1.534	7.74	2.71	0.20
1.688	3856.63	959.33	99.80