



Agilent Technologies

Sample name: M58687-KX2-361-02

Instrument: A012

Inj. volume: 4

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

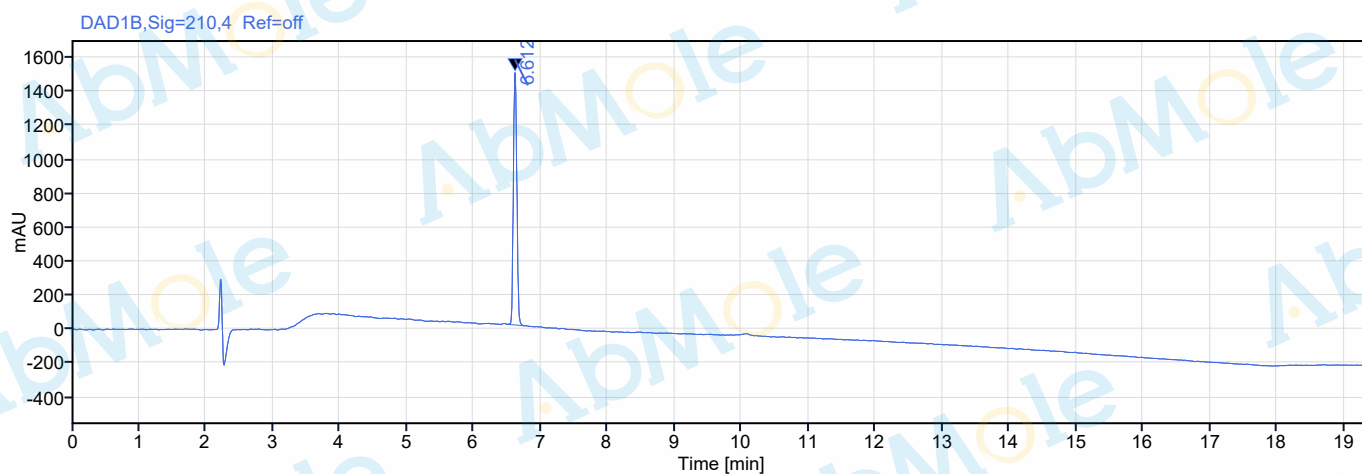

Signal: DAD1B,Sig=210,4 Ref=off

RT [min]	Area	Height	Area%
6.612	5413.19	1491.97	100.00