



Agilent Technologies

Sample name: M5944-Ruxolitinib phosphate-02

Injection date:

Instrument: A010

Location:

Inj. volume: 1.5


Type:

Acq. method: HPLC

Sample amount:

Processing method:

Manually modified:

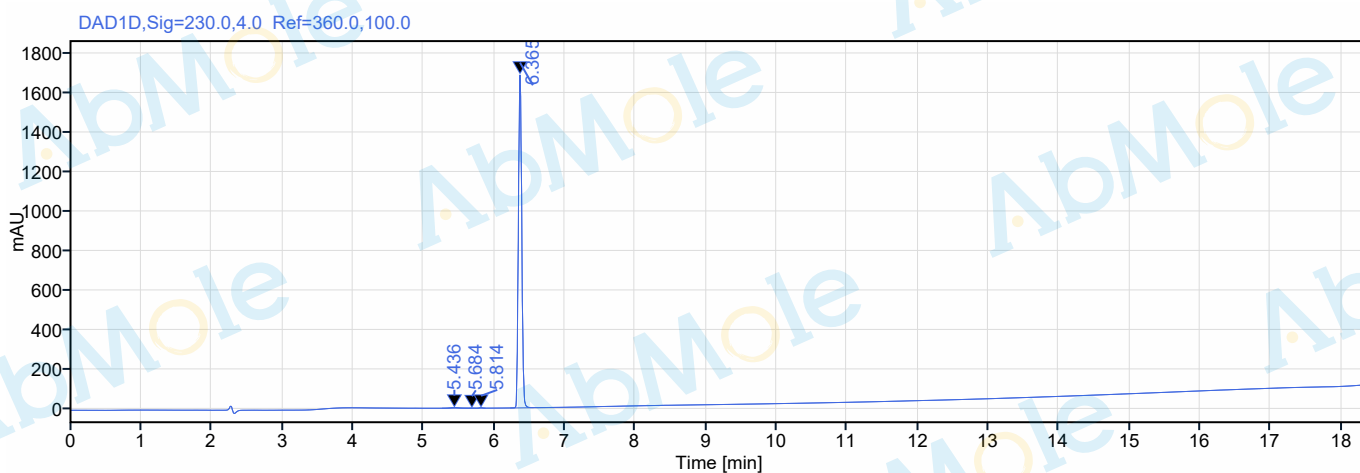

Signal: DAD1D,Sig=230.0,4.0 Ref=360.0,100.0

RT [min]	Type	Width [min]	Area	Height	Area%
5.436	MB m	0.37	26.12	3.19	0.47
5.684	MM m	0.11	1.25	0.45	0.02
5.814	BB	0.13	7.41	2.56	0.13
6.365	BB	0.33	5566.47	1682.63	99.38