


=====

Acq. Operator	: admin	
Sample Operator	: M5966-Sivelestat sodium tetrahydrate-01	
Acq. Instrument	: 3	Location : P1-A-06
		Inj : 1
		Inj Volume : 0.100 µl
Different Inj Volume from Sample Entry!	Actual Inj Volume	: 3.000 µl

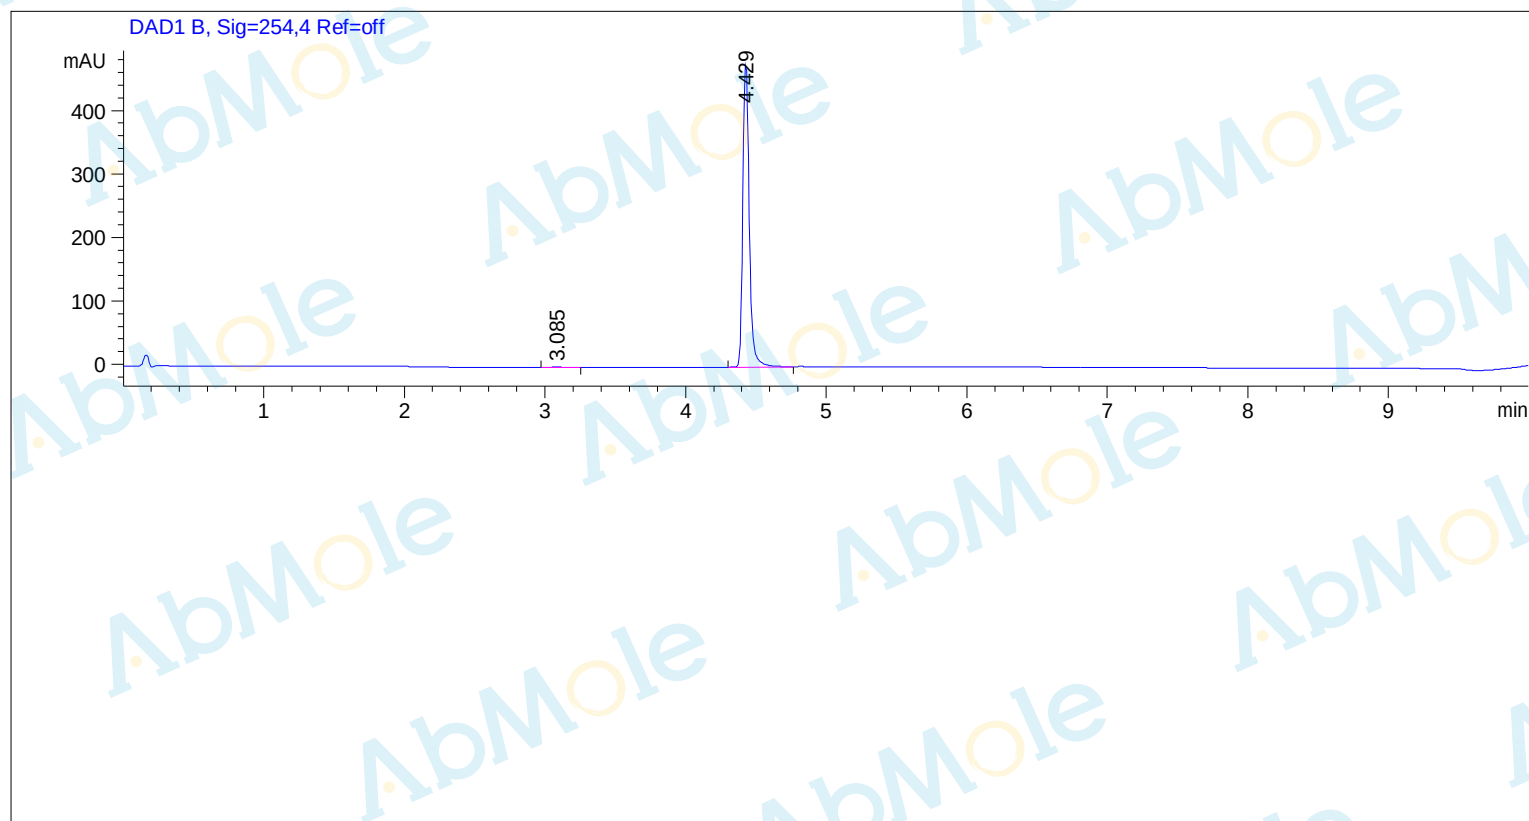

=====
Area Percent Report
=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 2: DAD1 B, Sig=254,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	3.085	BB	0.0680	5.85663	1.31280	0.3789
2	4.429	BB	0.0496	1539.76257	477.17352	99.6211

Totals : 1545.61920 478.48632