



Agilent Technologies

Sample name: M6298-Sodium tartrate-02

Instrument: A012

Inj. volume: 10

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

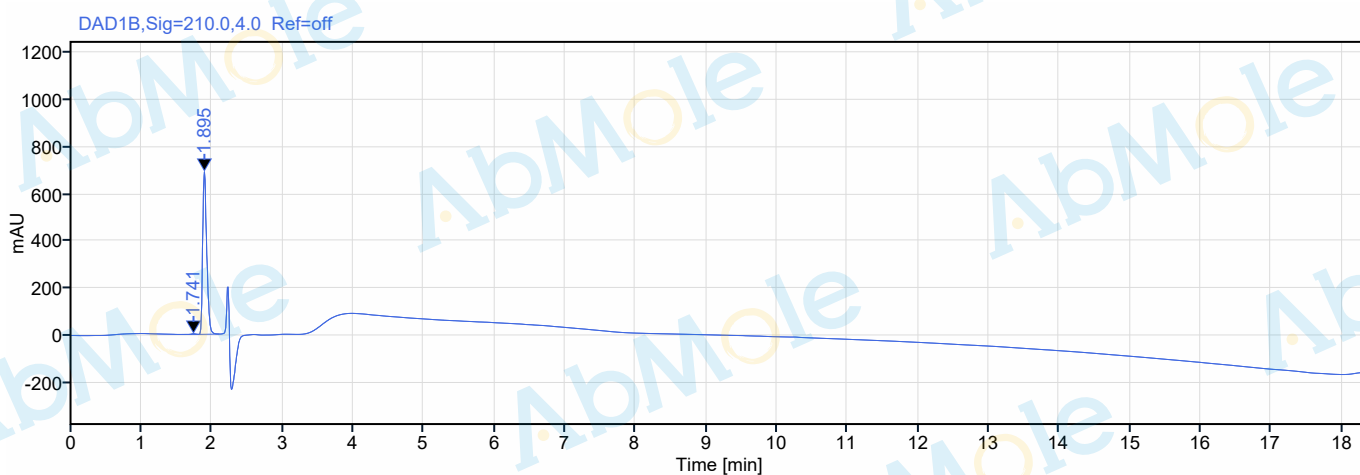

Signal: DAD1B,Sig=210.0,4.0 Ref=off

RT [min]	Area	Height	Area%
1.741	9.47	2.69	0.34
1.895	2743.53	691.32	99.66