



Agilent Technologies

Sample name: M6547-BX 471-02

Instrument: A010

Inj. volume: 3

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

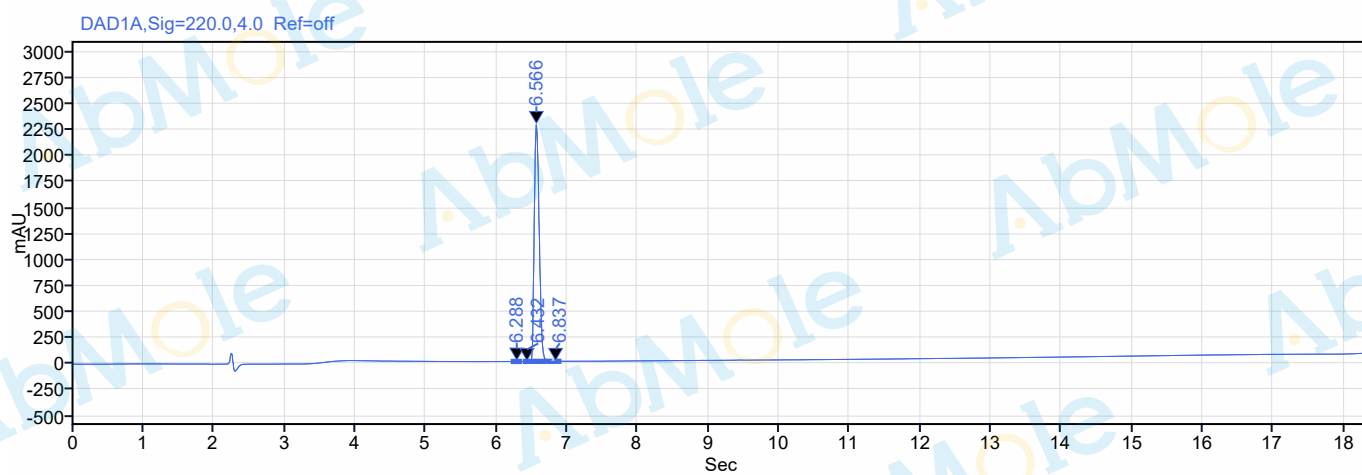

Signal: DAD1A, Sig=220.0, 4.0 Ref=off

RT [min]	Peak Resolution USP	Area	Height	Area%
6.288		18.0	5.9	0.163
6.432		3.2	1.0	0.029
6.566		11047.2	2280.5	99.763
6.837		5.0	1.3	0.045