



Agilent Technologies

Sample name: M6787-Harmine-02

Instrument: A012

Inj. volume: 2

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

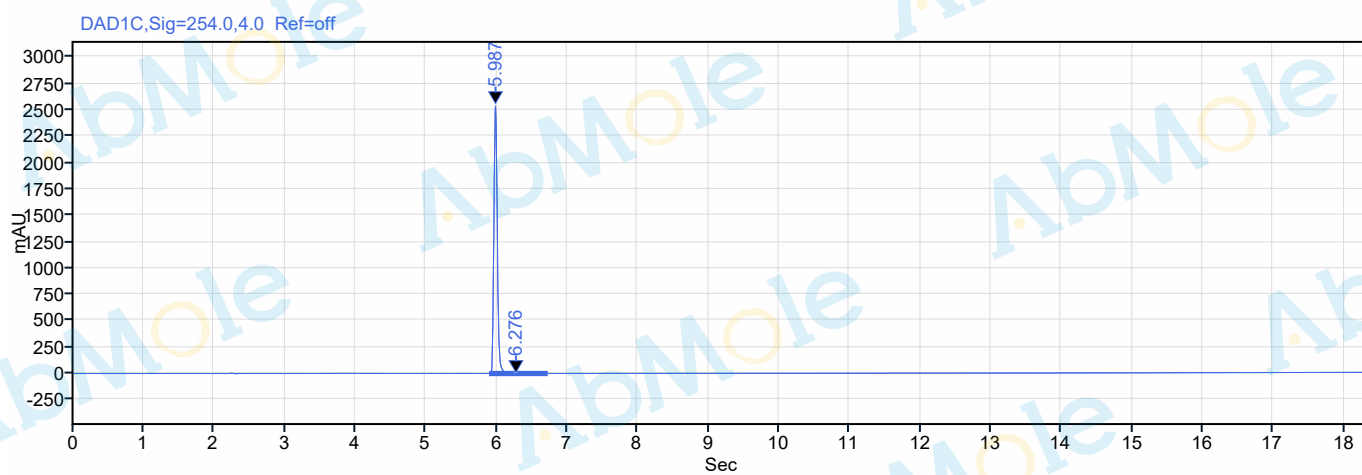

Signal: DAD1C,Sig=254.0,4.0 Ref=off

RT [min]	Peak Resolution USP	Width [min]	Area	Height	Area%
5.987		0.38	8623.1	2555.6	99.89
6.276		0.45	9.9	1.3	0.11