



Agilent Technologies

Sample name: M7059-NSC-87877-02

Instrument: A010

Inj. volume: 3

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

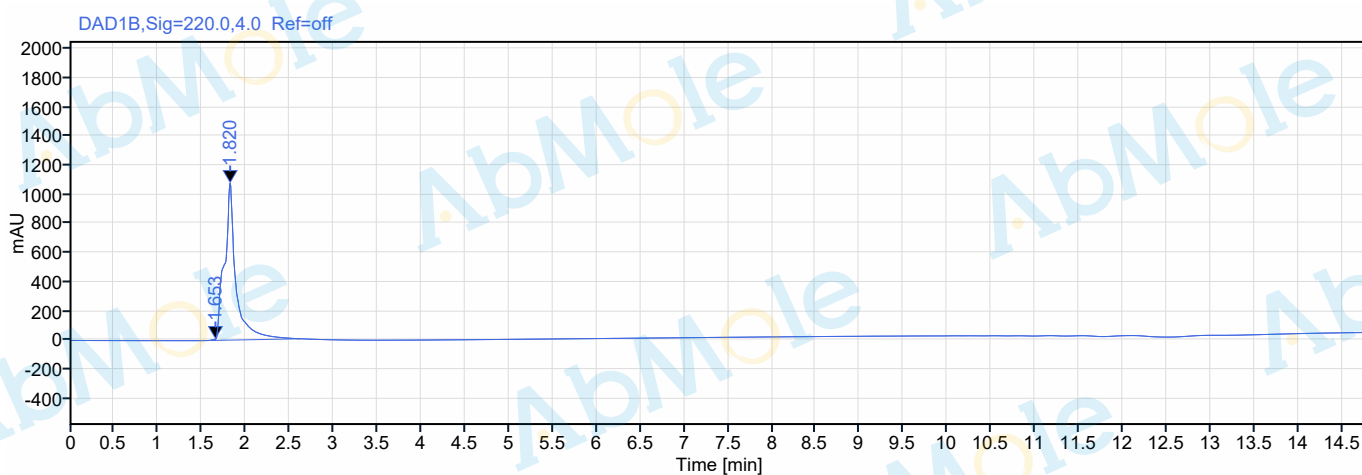

Signal: DAD1B, Sig=220.0, 4.0 Ref=off

RT [min]	Area	Height	Area%
1.653	17.87	7.46	0.18
1.820	9876.62	1076.71	99.82