



Agilent Technologies

Sample name: M7455-UK 5099-02

Instrument: A010

Inj. volume: 1

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

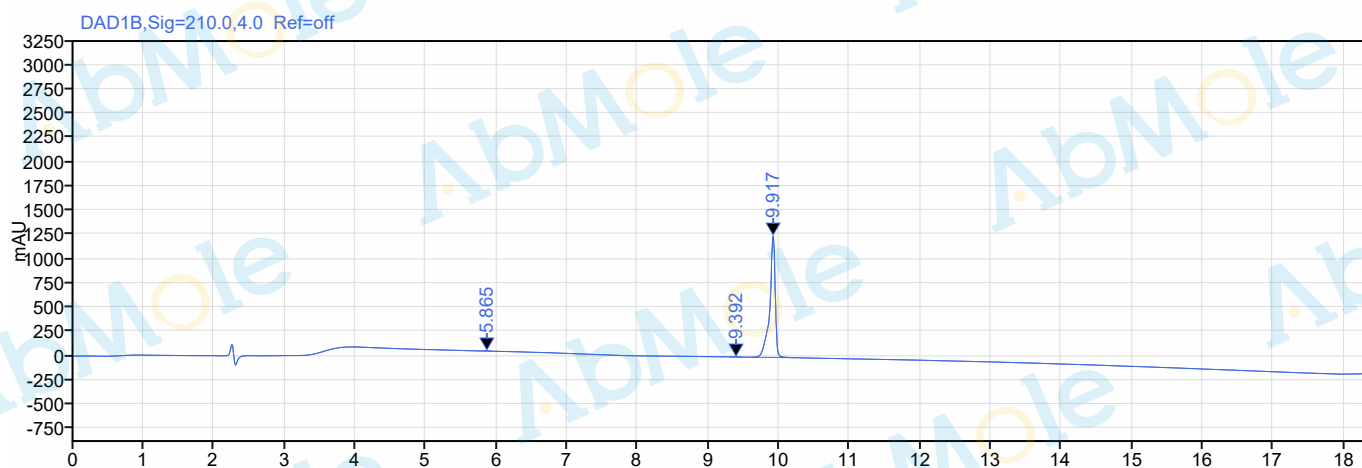

Signal: DAD1B,Sig=210.0,4.0 Ref=off

RT [min]	Area	Height	Area%
5.865	9.35	3.29	0.14
9.392	5.18	1.17	0.08
9.917	6787.67	1253.44	99.79