



Agilent Technologies

Sample name: M7576-Importazole-02

Instrument: A010

Inj. volume: 2

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

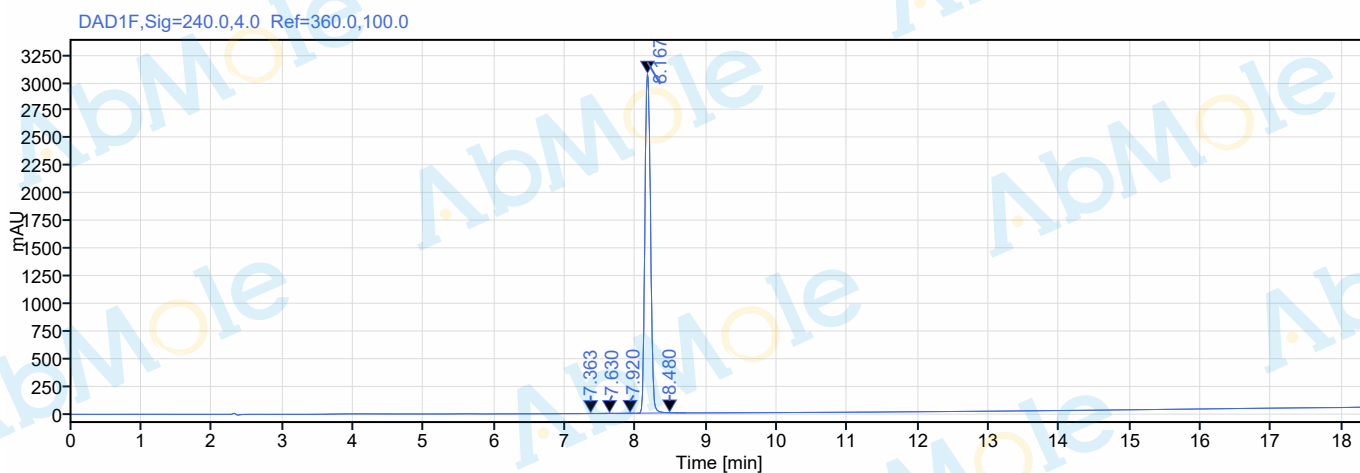

Signal: DAD1F,Sig=240.0,4.0 Ref=360.0,100.0

RT [min]	Type	Width [min]	Area	Height	Area%
7.363	MM m	0.14	4.18	0.88	0.02
7.630	MM m	0.17	3.11	0.41	0.02
7.920	MM m	0.12	1.78	0.55	0.01
8.167	MM m	0.45	16875.84	3075.34	99.91
8.480	MM m	0.24	6.45	1.11	0.04