



Sample name: M7874-KH7-01

Instrument: A010

Inj. volume: 3

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

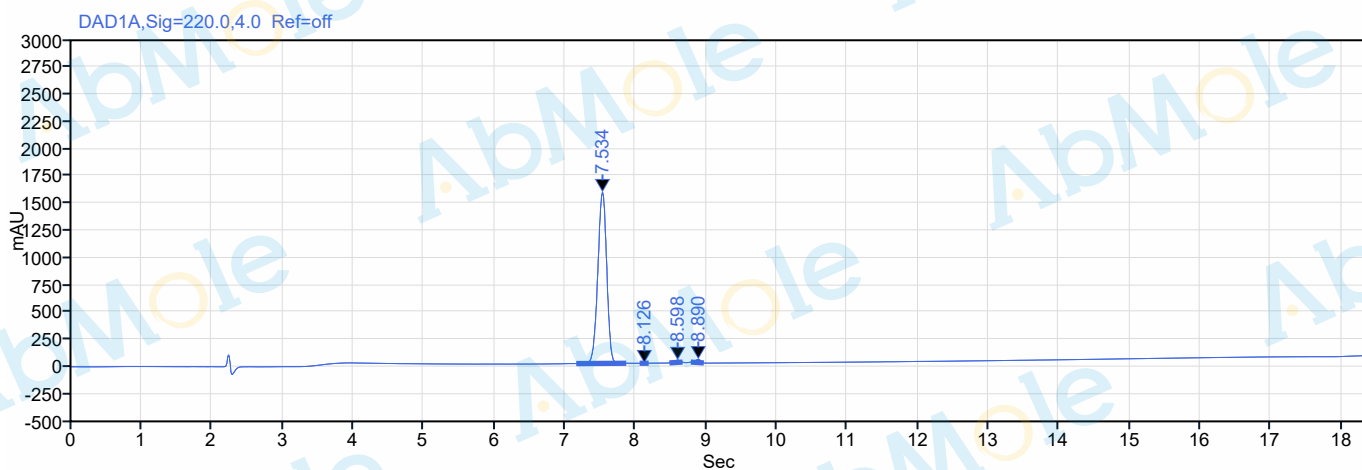

Signal: DAD1A,Sig=220.0,4.0 Ref=off

| RT [min] | Peak Resolution USP | Area | Height | Area% |
|----------|---------------------|---------|--------|--------|
| 7.534 | | 13762.5 | 1572.4 | 98.054 |
| 8.126 | | 1.7 | 0.5 | 0.012 |
| 8.598 | | 118.0 | 21.1 | 0.841 |
| 8.890 | | 153.5 | 30.2 | 1.094 |