



Agilent Technologies

Sample name: M8221-Trapidil-01

Instrument: A010

Inj. volume: 1

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

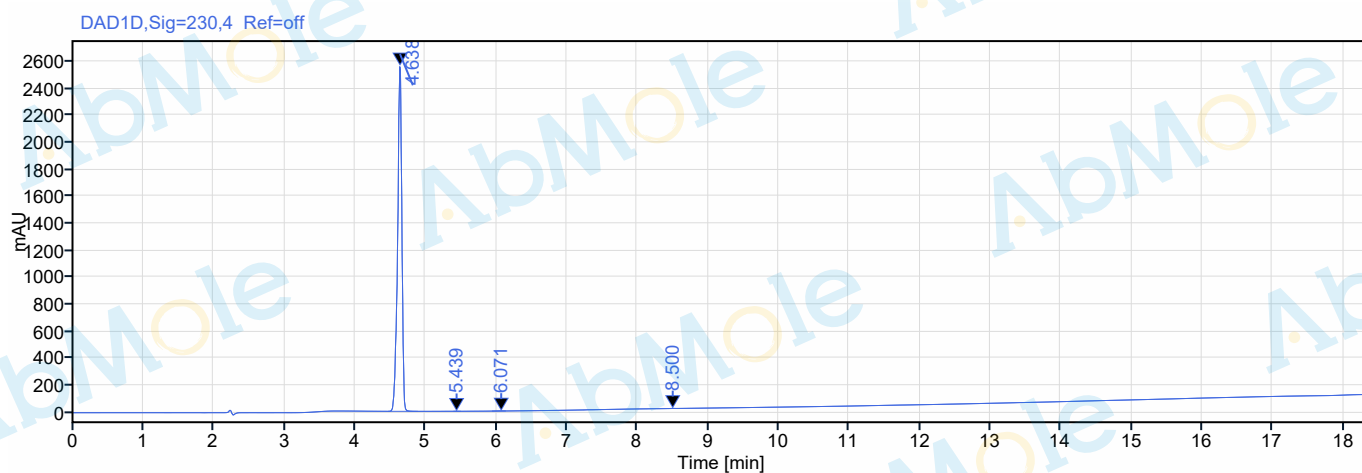

Signal: DAD1D,Sig=230,4 Ref=off

| RT [min] | Type | Width [min] | Area     | Height  | Area% |
|----------|------|-------------|----------|---------|-------|
| 4.638    | BM m | 0.42        | 10790.82 | 2558.49 | 99.94 |
| 5.439    | MM m | 0.10        | 1.32     | 0.50    | 0.01  |
| 6.071    | MM m | 0.20        | 2.55     | 0.41    | 0.02  |
| 8.500    | MM m | 0.11        | 2.33     | 0.72    | 0.02  |