

Acq. Operator : admin

Sample Operator : Chemist-1


Acq. Instrument : 3

Location : P2-E-06

Inj : 1

Inj Volume : 0.100 µl

Different Inj Volume from Sample Entry! Actual Inj Volume : 4.000 µl

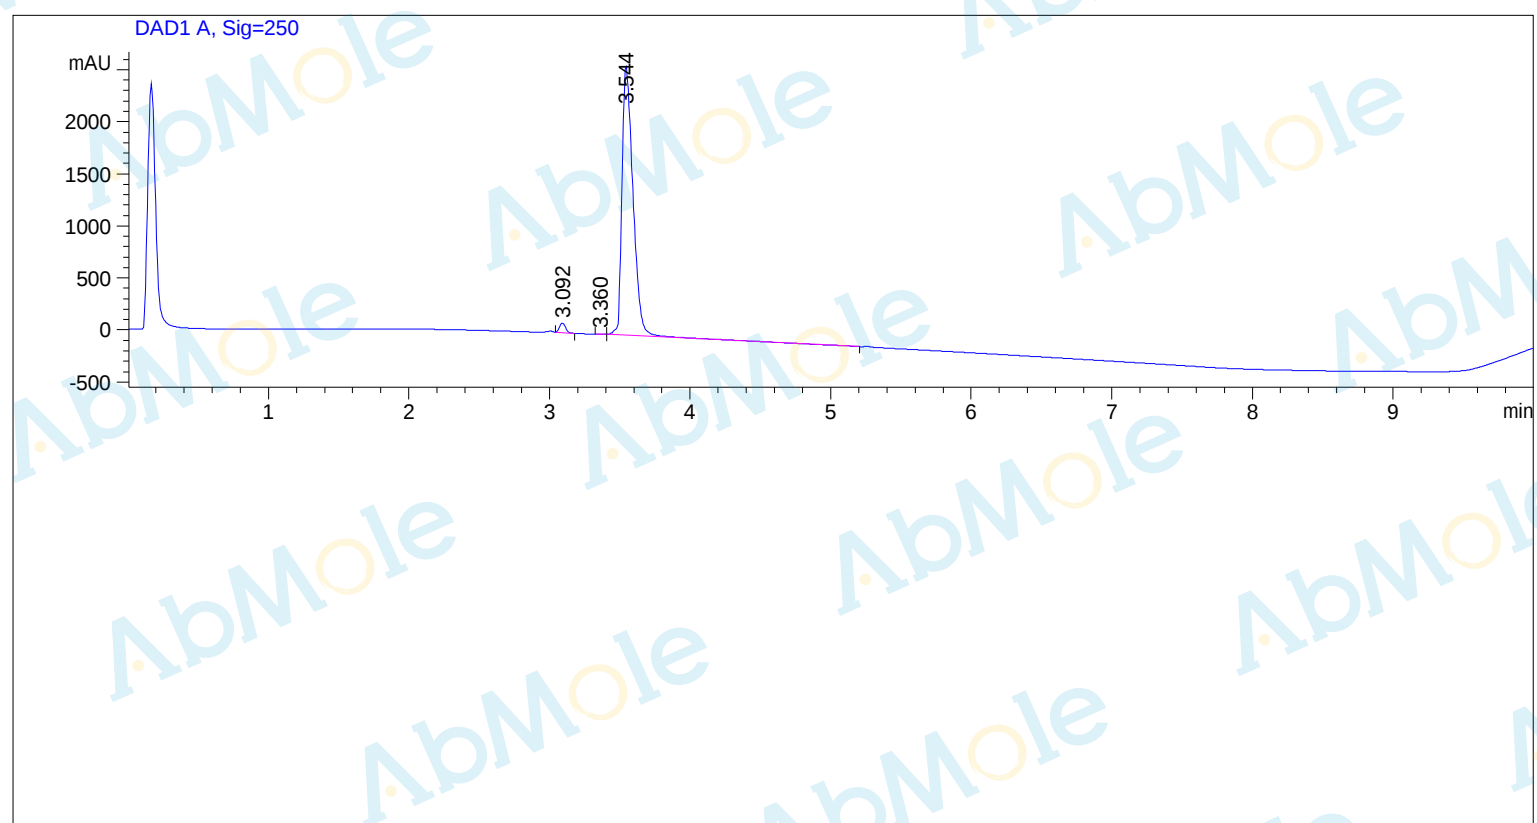

Area Percent Report

Sorted By : Signal

Multiplier : 1.0000

Dilution : 1.0000

Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 A, Sig=250,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	3.092	BB	0.0459	264.60367	90.98268	1.8298
2	3.360	BB	0.0416	5.68546	2.23758	0.0393
3	3.544	BB	0.0841	1.41904e4	2584.30786	98.1309

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
Totals :				1.44607e4	2677.52813	