




Agilent Technologies

Sample name: M8424-KC7F2-01
Instrument: 5
Inj. volume: HPLC
Acq. method:
Processing method:
Manually modified:

Injection date:
Location:
Type:
Sample amount:

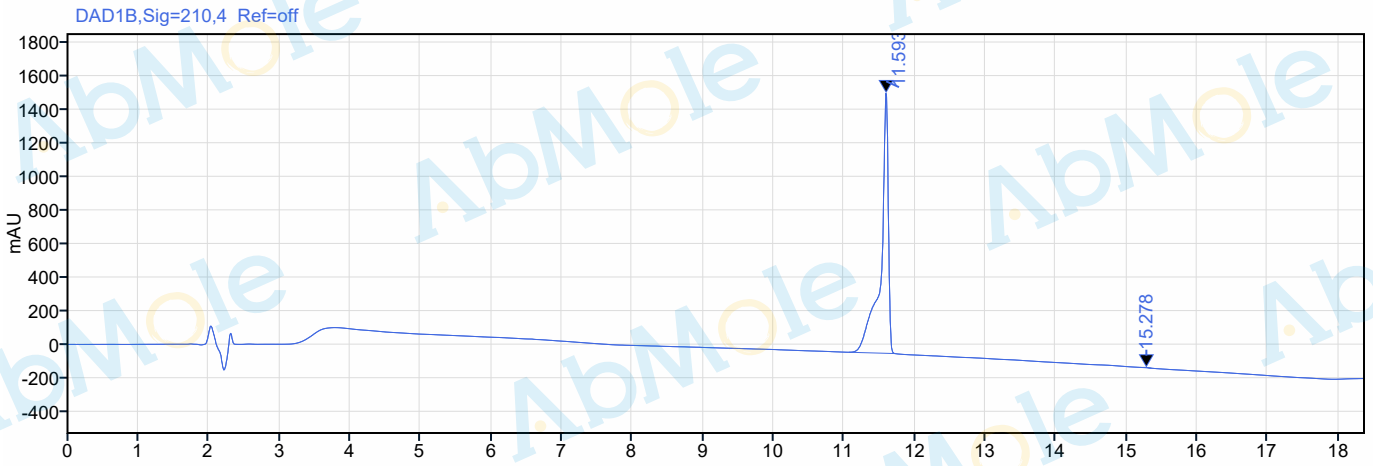

Signal: DAD1B, Sig=210,4 Ref=off

RT [min]	Area	Height	Area%
11.593	11593.88	1548.94	99.91
15.278	10.00	2.15	0.09
Sum	11603.88		