




Agilent Technologies

Sample name: M8873-D-Luciferin potassium salt-18 Injection date:
Instrument: A010 Location:
Inj. volume: 1 Type:
Acq. method: HPLC Sample amount:
Processing method:
Manually modified:

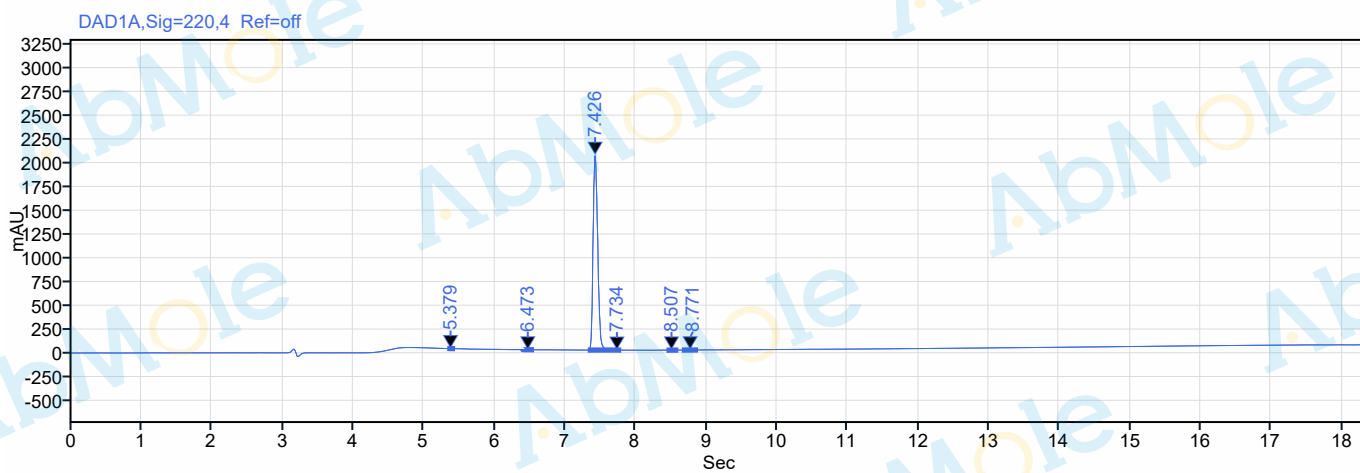

Signal: DAD1A, Sig=220,4 Ref=off

RT [min]	Peak Resolution USP	Area	Height	Area%
5.379		8.1	2.7	0.086
6.473		5.7	1.2	0.061
7.426		9277.8	2054.0	99.289
7.734		7.5	2.4	0.081
8.507		21.1	4.4	0.226
8.771		24.1	5.2	0.257