


=====

Acq. Operator	: admin	Location	: P1-C-03
Sample Operator	: 1	Inj	: 1
Acq. Instrument	: 3	Inj Volume	: 0.100 µl
Sample Name	: M8924-Daprodustat-02	Actual Inj Volume	: 3.000 µl

Different Inj Volume from Sample Entry!

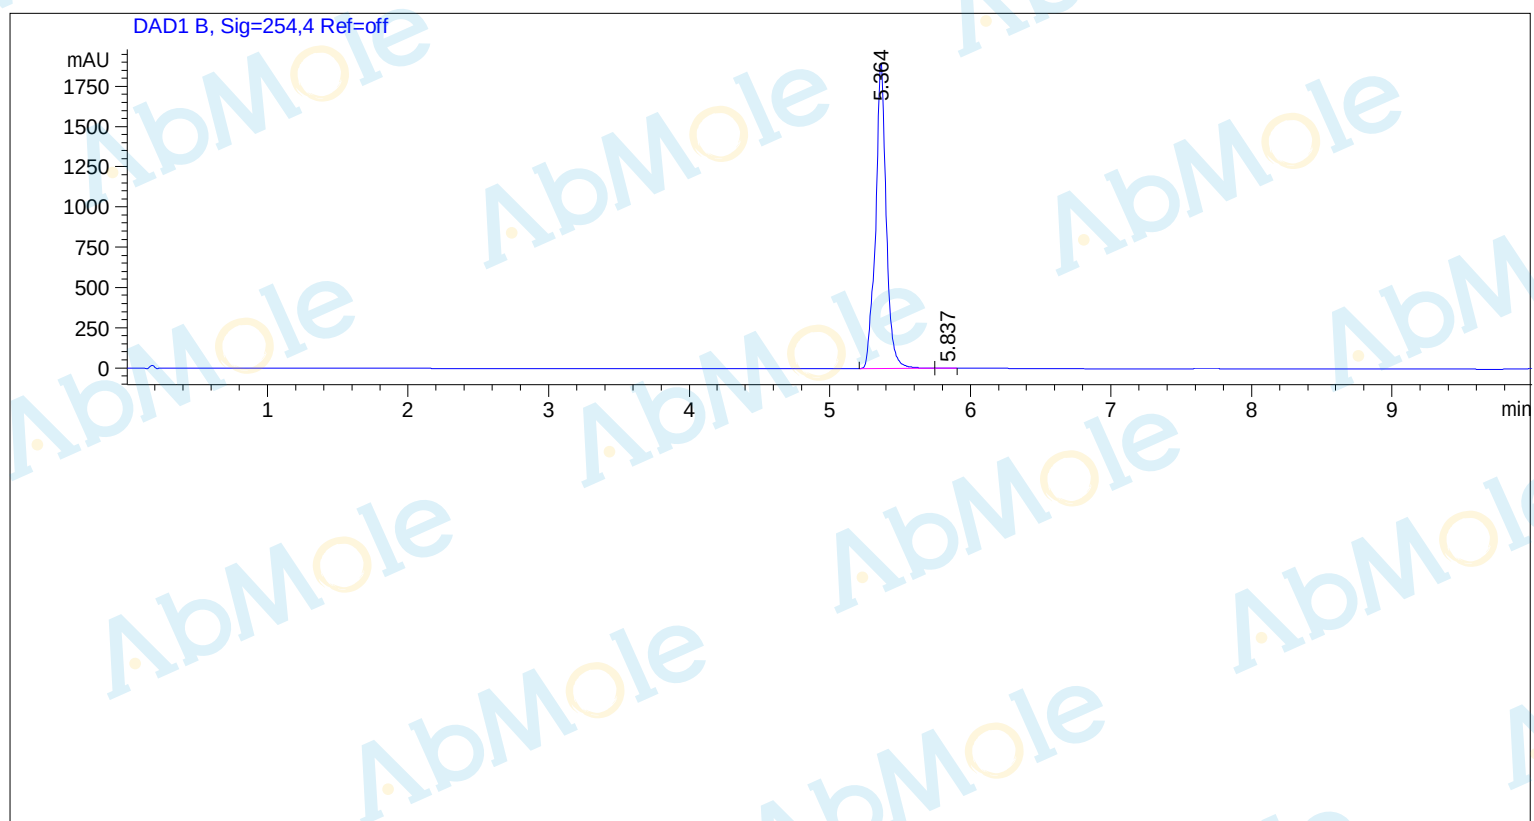

=====
Area Percent Report
=====

Sorted By	:	Signal
Multiplier	:	1.0000
Dilution	:	1.0000

Do not use Multiplier & Dilution Factor with ISTDs

Signal 2: DAD1 B, Sig=254,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	5.364	BB	0.0749	9935.30859	1902.71216	99.9431
2	5.837	BB	0.0603	5.66017	1.42653	0.0569

Totals : 9940.96876 1904.13868