


```

=====
Acq. Operator   : SYSTEM                      Seq. Line :    6
Acq. Instrument : 0                        Location  : P2-A-06
Sample Name     : M8978-3-TYP-03           Inj       :    1
                                                Inj Volume: 1.000 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 3.000 µl
=====

```

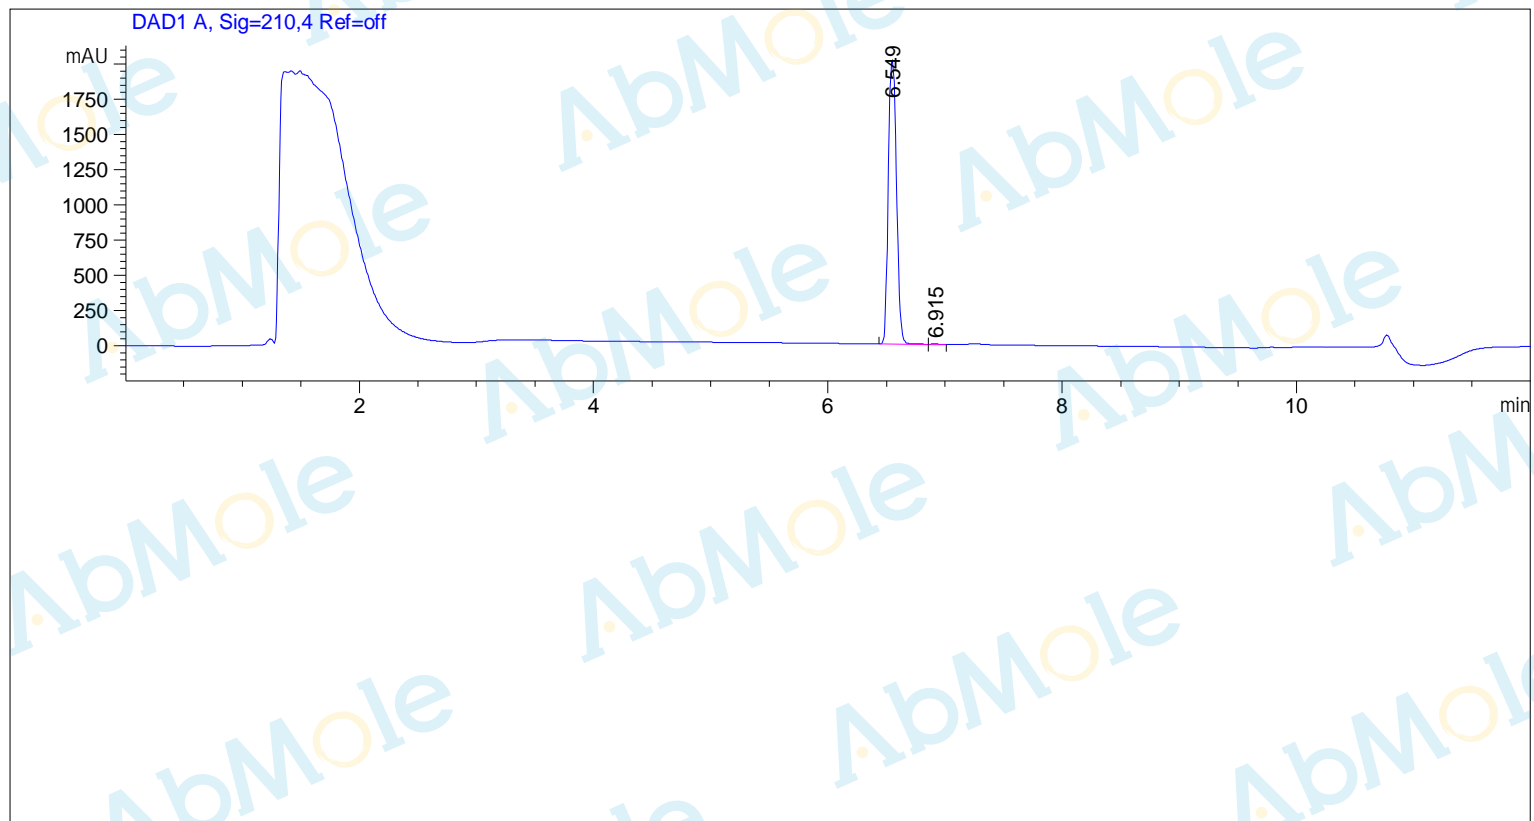

```

=====
                          Area Percent Report
=====

```

```

Sorted By       :      Signal
Multiplier      :      1.0000
Dilution        :      1.0000
Use Multiplier & Dilution Factor with ISTDs

```

Signal 1: DAD1 A, Sig=210,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	6.549	BB	0.0787	9805.51660	2017.32910	99.8976
2	6.915	BB	0.0560	10.05068	2.79508	0.1024

Totals : 9815.56728 2020.12418