



Agilent Technologies

Sample name: M9133-AKBA-02

Instrument: A010

Inj. volume: 6

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

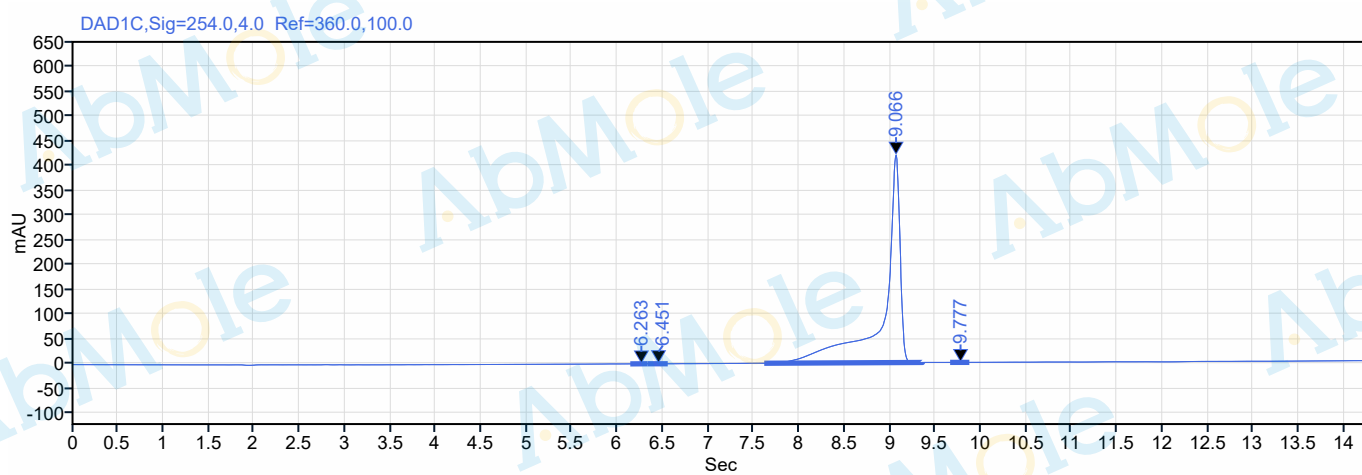

Signal: DAD1C,Sig=254.0,4.0 Ref=360.0,100.0

RT [min]	Peak Resolution USP	Width [min]	Area	Height	Area%
6.263		0.19	0.8	0.2	0.02
6.451		0.22	3.6	0.6	0.07
9.066		1.74	5158.4	418.3	99.89
9.777		0.21	1.2	0.2	0.02