



Agilent Technologies

Sample name: M9210-Ampicillin-02

Instrument: A010

Inj. volume: 2

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

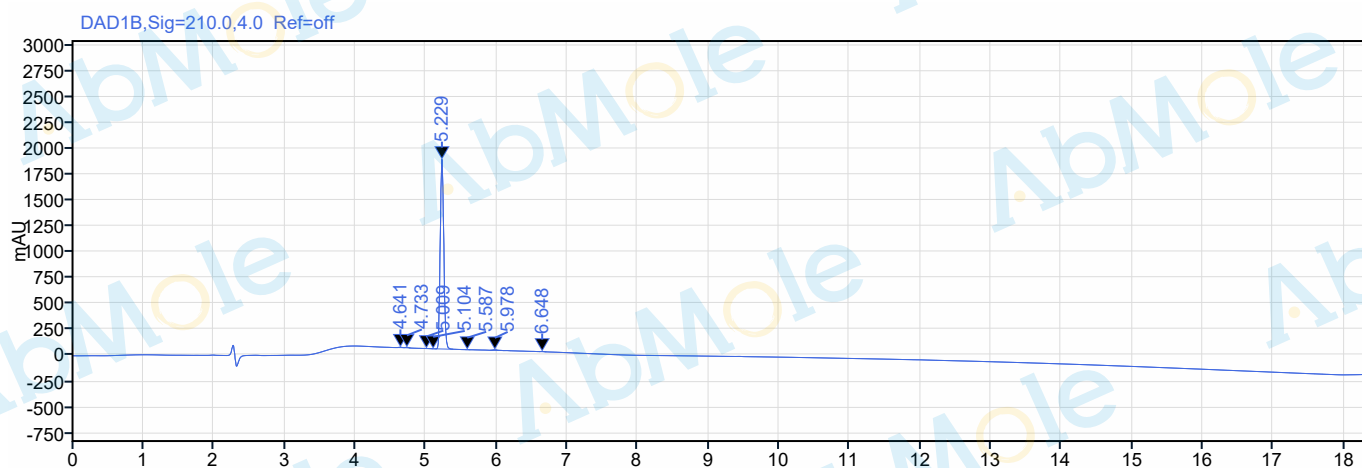

Signal: DAD1B,Sig=210.0,4.0 Ref=off

RT [min]	Area	Height	Area%
4.641	9.95	3.71	0.15
4.733	14.22	5.02	0.22
5.009	5.78	1.10	0.09
5.104	0.00	0.00	0.00
5.229	6447.87	1835.68	99.00
5.587	1.53	0.58	0.02
5.978	25.64	5.98	0.39
6.648	7.90	2.39	0.12