

M9302-CBL0137-01-LCMS

Sample Information

LCMS


Acquired by : System Administrator
Sample Name : M9302-CBL0137-01
Method File : B 5%-95%-P-new - 2.6min.lcm

Date Acquired : 2021/7/27 10:41:45
Injection Volume : 2
Vial : 35


Column : Waters SunFire C18 50*4.6mm 5um 2.000ml/min 2.6min
Pump A : 0.1% FA and 10% ACN in H2O
Pump B : 0.1% FA and 10% H2O in ACN

Chromatogram


mAU

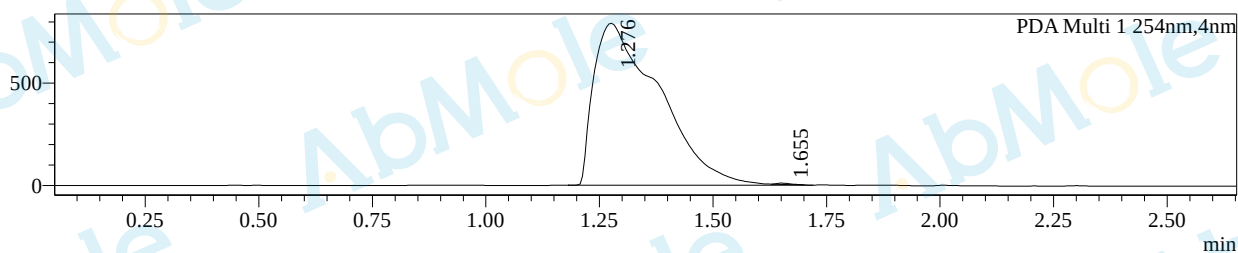

mAU

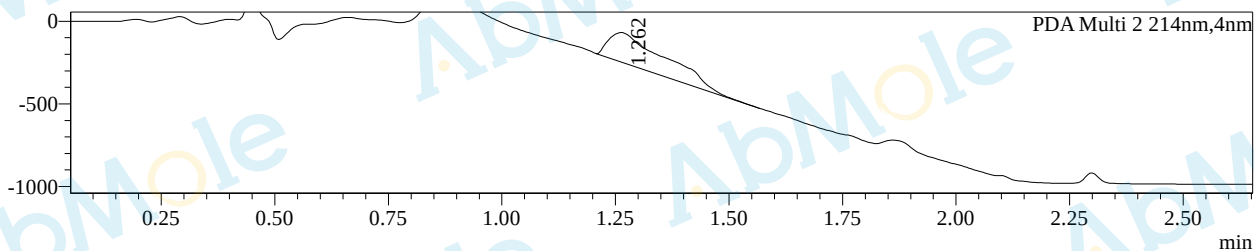

段号1

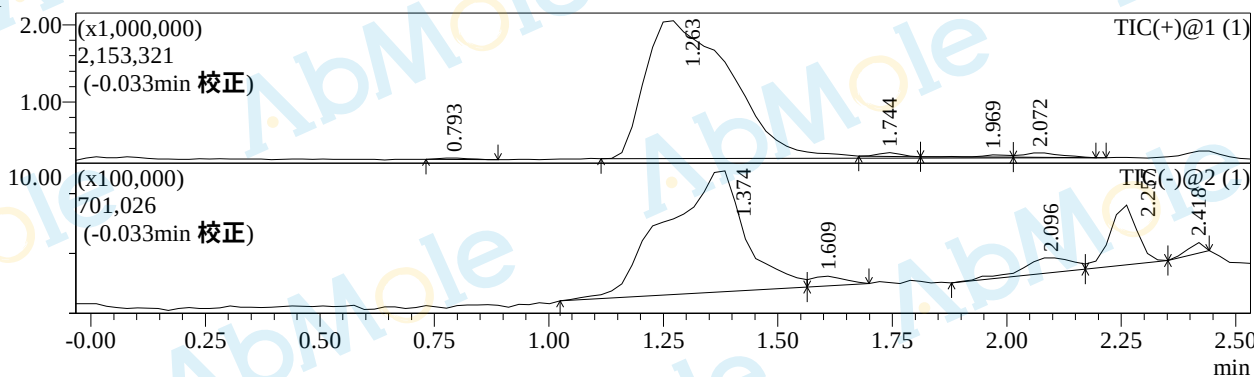

Integration Results for DAD

PDA Ch1 254nm


Peak#	Ret. Time	Height	Area	Area%
1	1.276	792437	7958597	99.853
2	1.655	6038	11698	0.147
总计		798475	7970295	100.000

PDA Ch2 214nm


Peak#	Ret. Time	Height	Area	Area%
1	1.262	178375	1662377	100.000
总计		178375	1662377	100.000

Mass Spectrum


Rt=0.777min 正

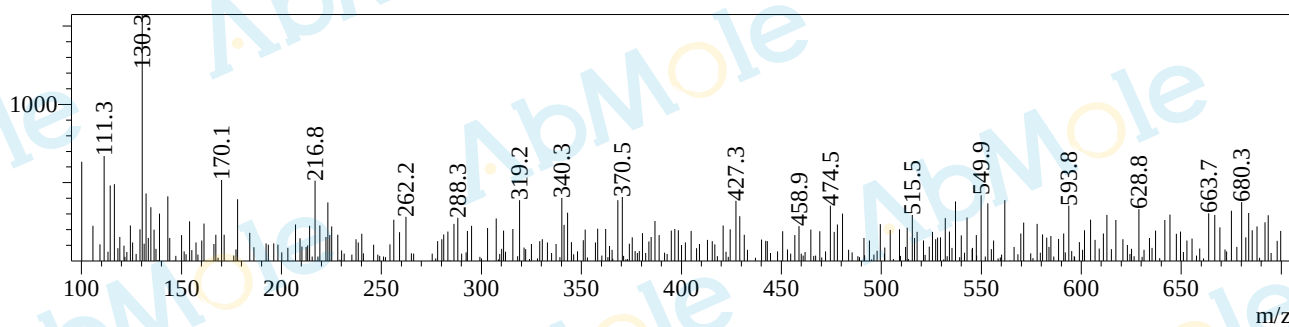


Rt=1.249min 正

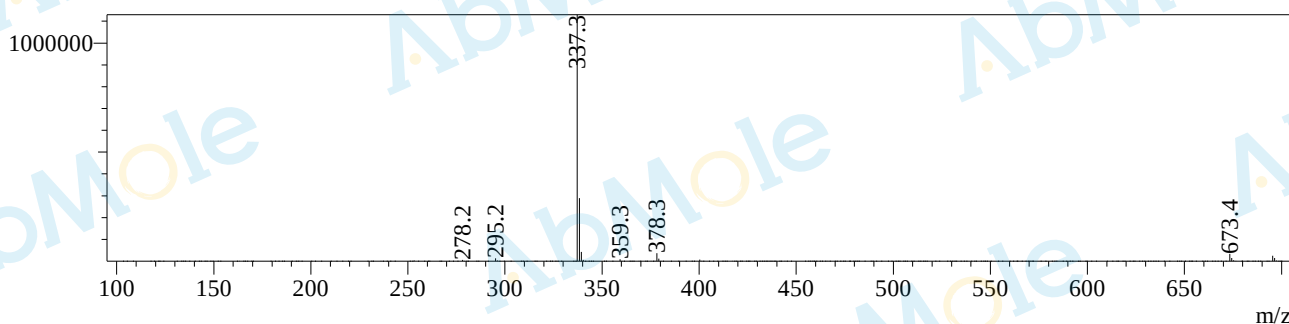


Rt=1.367min 负

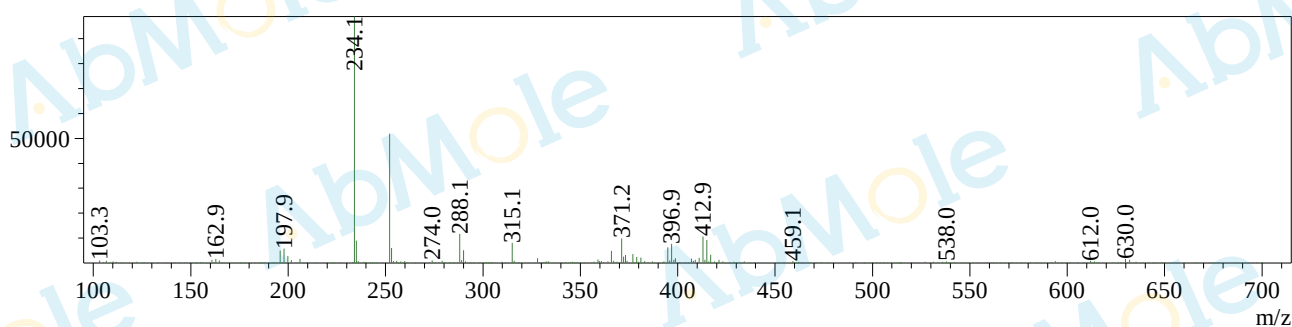


Rt=1.615min 负

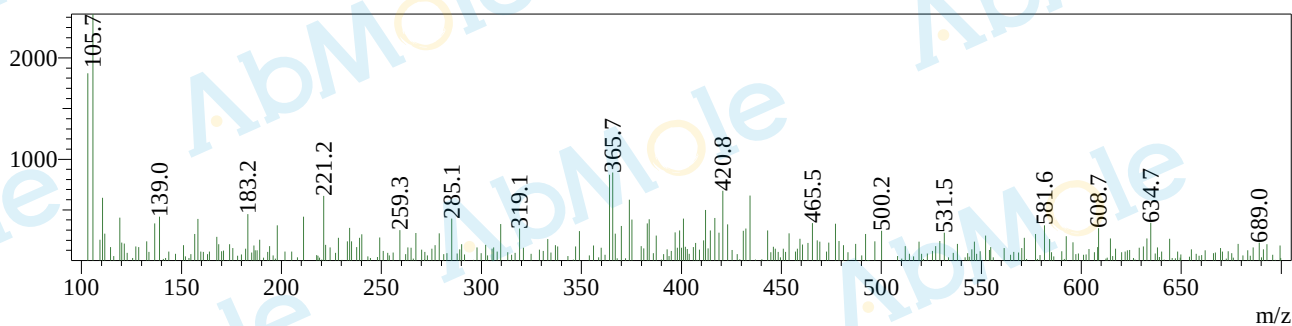


Rt=1.722min 正

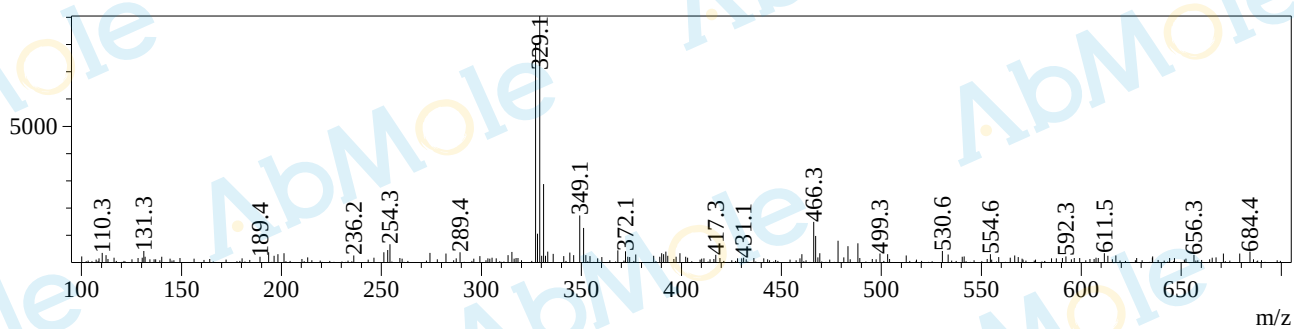


Rt=1.969min 正

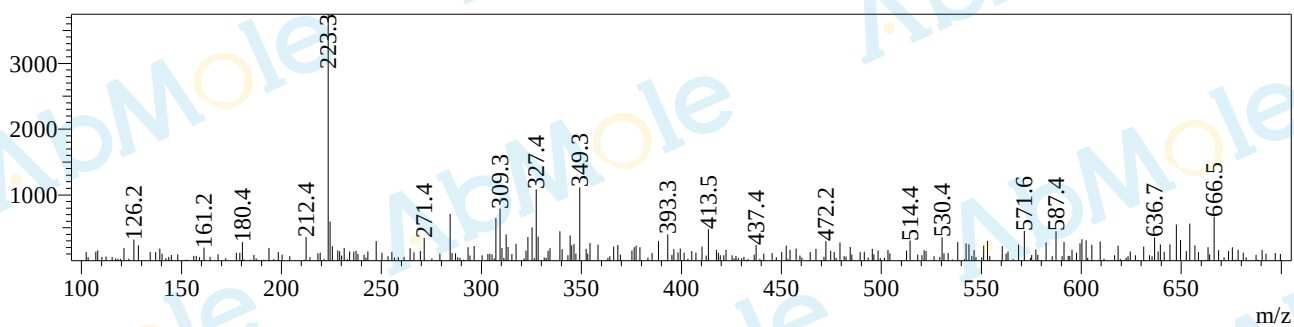


Rt=2.059min 正

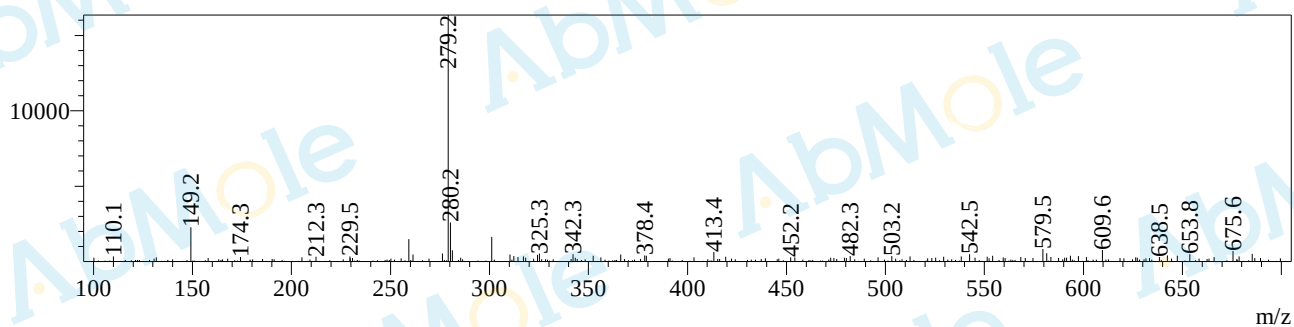

Rt=2.087min 负

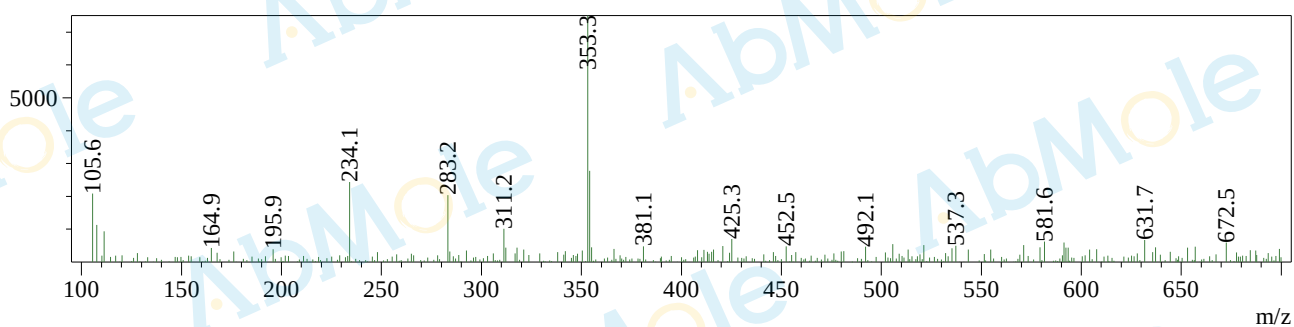

Rt=2.245min 负

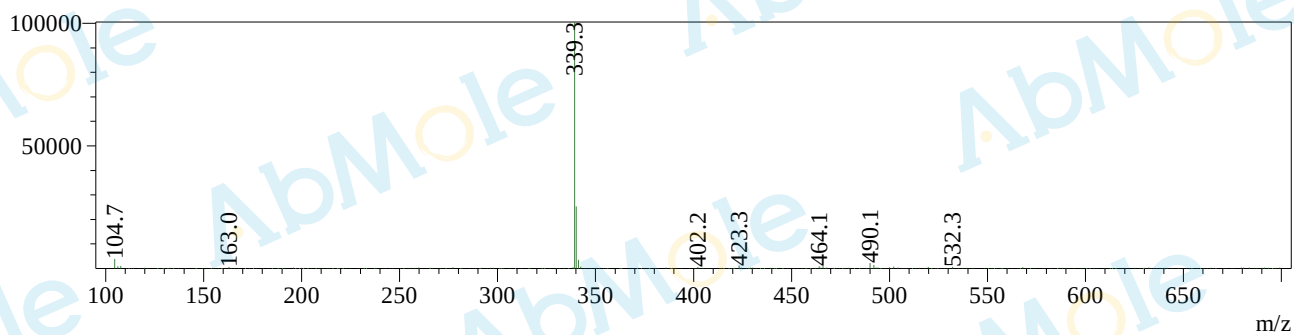

Rt=2.402min 负

