



Agilent Technologies

Sample name: M9358-ITE-02

Instrument: A010

Inj. volume: 1.5

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

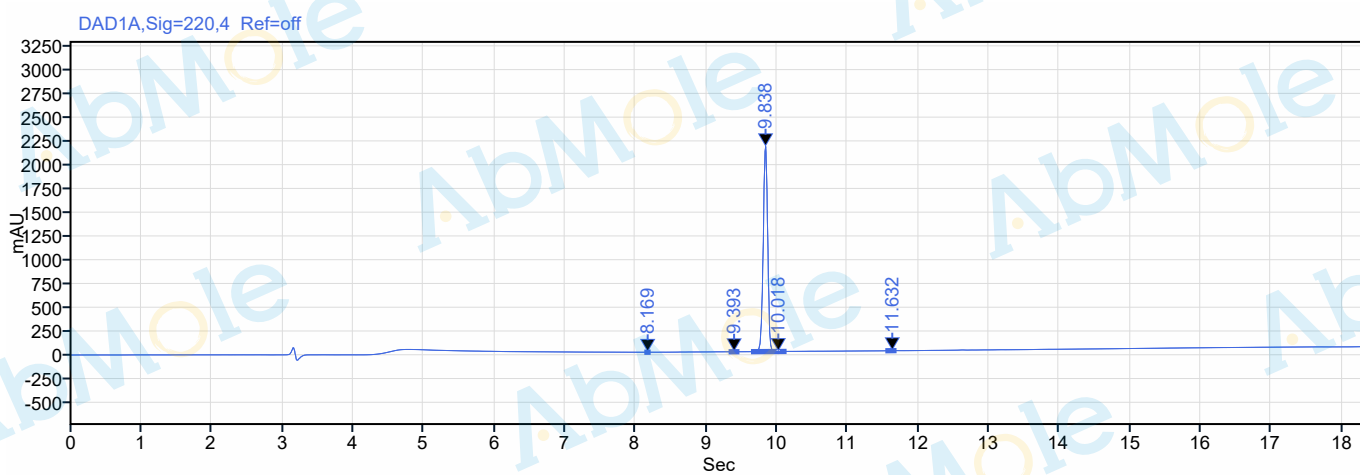

Signal: DAD1A,Sig=220,4 Ref=off

RT [min]	Peak Resolution USP	Area	Height	Area%
8.169		2.1	0.8	0.023
9.393		6.1	1.6	0.064
9.838		9492.5	2158.7	99.803
10.018		4.6	1.4	0.048
11.632		5.9	1.4	0.062