


=====
Acq. Operator : admin
Sample Operator : M9512-PLX5622-05
Acq. Instrument : 3

Location : P1-E-10

Inj : 1

Inj Volume : 0.100 µl

Different Inj Volume from Sample Entry! Actual Inj Volume : 3.000 µl

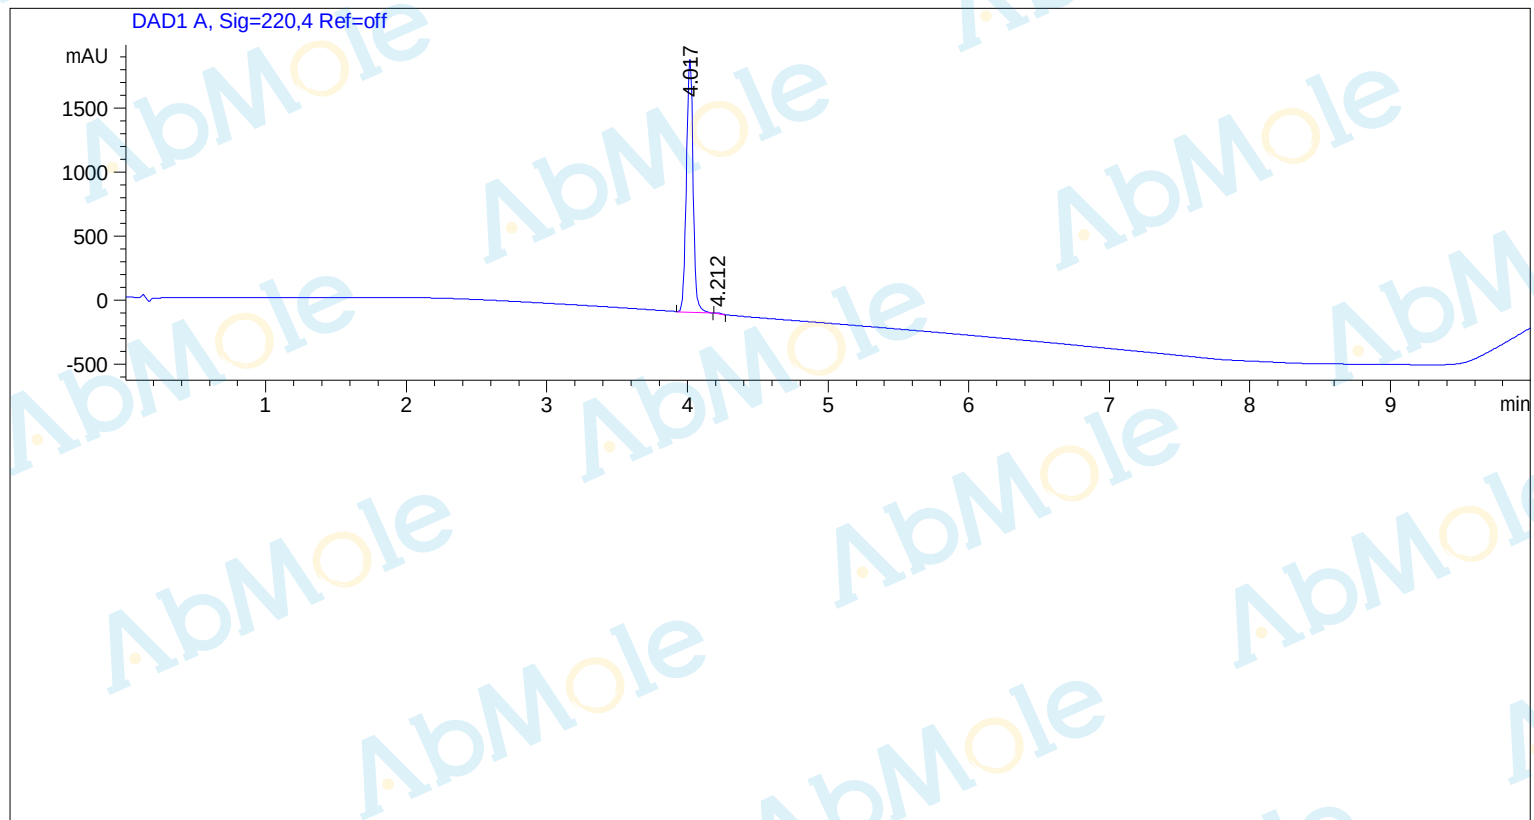

=====
Area Percent Report
=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 A, Sig=220,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	4.017	BB	0.0527	6539.38135	1971.71411	99.7613
2	4.212	BB	0.0441	15.64399	5.69228	0.2387

Totals :

6555.02533 1977.40639