



Agilent Technologies

Sample name: M9522-SRI-011381-01

Instrument: A010

Inj. volume: 5

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

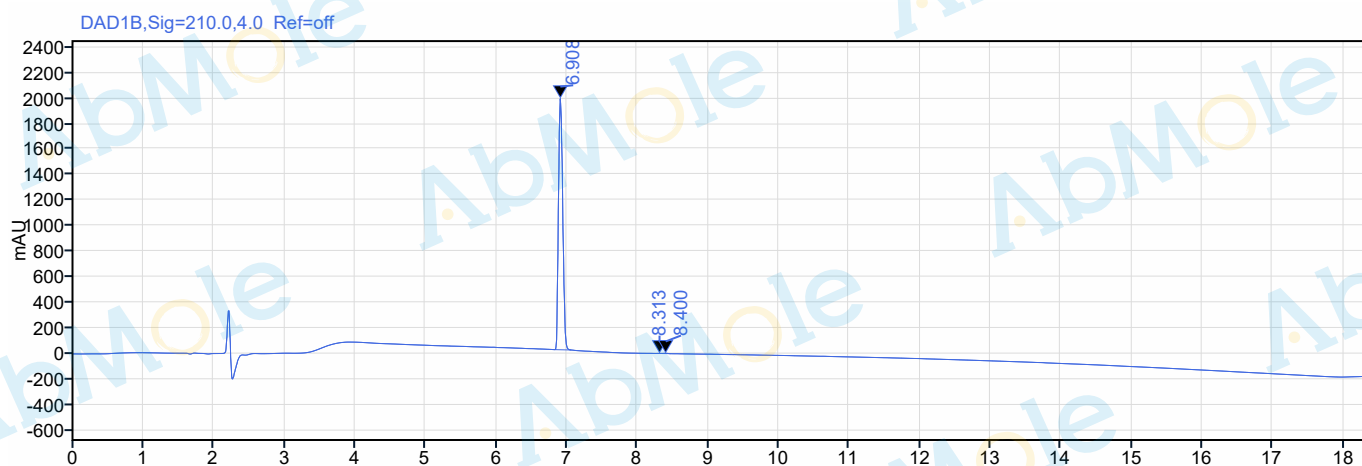

Signal: DAD1B,Sig=210.0,4.0 Ref=off

RT [min]	Area	Height	Area%
6.908	8282.81	1968.16	99.88
8.313	2.01	0.59	0.02
8.400	8.29	2.10	0.10