




Sample name: M9621-KIRA6-01  
Instrument: A010  
Inj. volume: 3  
Acq. method: HPLC  
Processing method:  
Manually modified:

Injection date:  
Location:  
Type:  
Sample amount:

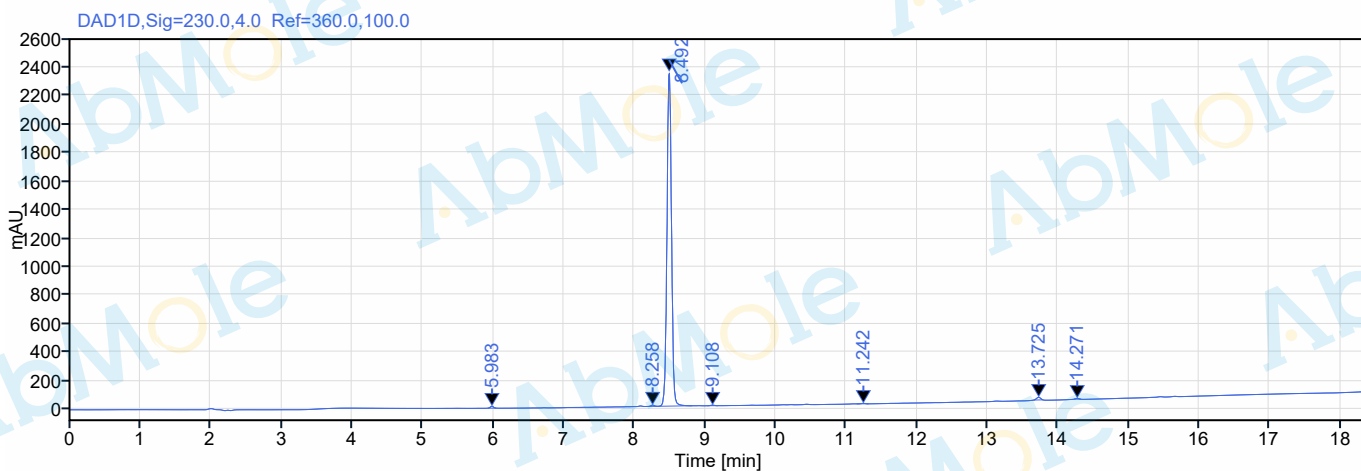

Signal: DAD1D, Sig=230.0,4.0 Ref=360.0,100.0

RT [min]	Type	Width [min]	Area	Height	Area%
5.983	MM m	0.12	40.87	13.43	0.39
8.258	MB m	0.13	28.13	8.81	0.27
8.492	BM m	0.49	10393.56	2346.29	98.19
9.108	MV m	0.15	14.77	3.86	0.14
11.242	BB	0.17	13.56	3.39	0.13
13.725	MM m	0.13	74.50	18.75	0.70
14.271	MM m	0.10	19.36	5.98	0.18